

LBW4U

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

10/9/2020 15:50

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.056	0.0	0.082	
ICB1	0.615	0.0	0.000	
CCV1	249.485	0.0	0.213	
CCB1	0.680	0.0	0.000	
PB132247BL	0.539	0.0	0.000	
PB132247BS	94.873	0.0	0.081	
MIDPB132247	246.604	0.0	0.210	
L4214-12	2.885	0.0	0.002	
L4327-07	19.037	0.0	0.016	
L4327-07DUP	19.199	0.0	0.016	
L4327-07MS	53.717	0.0	0.046	
L4327-07MSD	53.551	0.0	0.045	
CCV2	247.651	0.0	0.211	
CCB2	0.423	0.0	0.000	

N	14
Mean	77.522
SD	98.0473
CV%	126.48

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AM

Instrument ID : Konelab

10/9/2020 10:01


Test Total CN

Accepted 10/9/2020 10:01

Factor 1170
 Bias 0

Coeff. of det. 0.999974

Errors

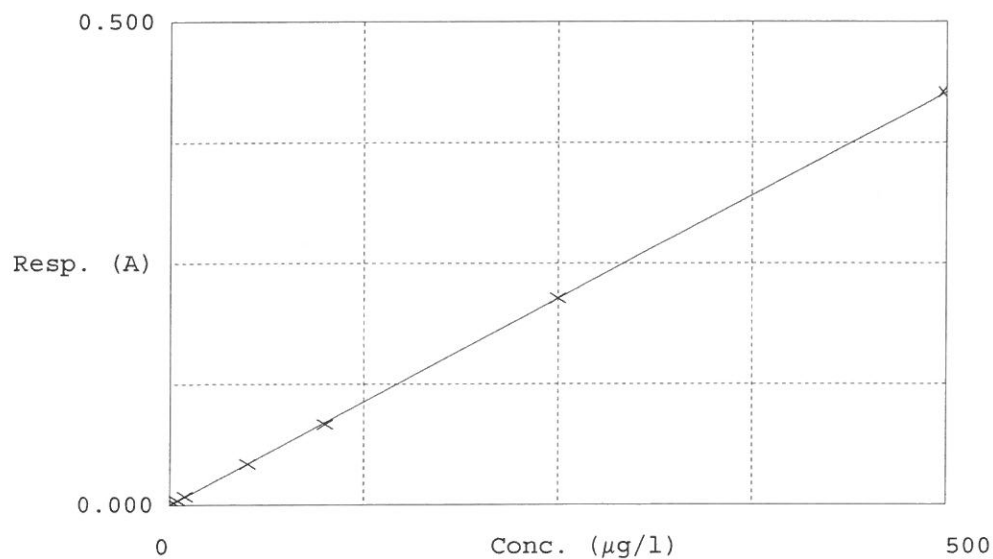

	Calibrator	Response	Calc. con.	Conc.	Errors

1	0.0PPBCN	0.000	0.3188	0.0000	
2	5.0PPBCN	0.004	5.3806	5.0000	
3	10PPBCN	0.009	10.8156	10.0000	
4	50PPBCN	0.042	49.8769	50.0000	
5	100PPBCN	0.083	97.9707	100.0000	
6	250PPBCN	0.214	250.4787	250.0000	
7	500PPBCN	0.427	500.1587	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri Oct 09 15:37:46 2020

Fri Oct 09 15:48:09 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.3188	µg/l	10/9/2020 10:00:43	
5.OPPBCN	A	Total CN	P	5.3806	µg/l	10/9/2020 10:00:44	
10PPBCN	A	Total CN	P	10.8156	µg/l	10/9/2020 10:00:45	
50PPBCN	A	Total CN	P	49.8769	µg/l	10/9/2020 10:00:46	
100PPBCN	A	Total CN	P	97.9707	µg/l	10/9/2020 10:00:47	
250PPBCN	A	Total CN	P	250.4787	µg/l	10/9/2020 10:00:48	
500PPBCN	A	Total CN	P	500.1587	µg/l	10/9/2020 10:00:49	
ICV1	S	Total CN	P	96.0561	µg/l	10/9/2020 15:37:47	
ICB1	S	Total CN	P	0.6151	µg/l	10/9/2020 15:37:48	
CCV1	S	Total CN	P	249.4849	µg/l	10/9/2020 15:37:51	
CCB1	S	Total CN	P	0.6798	µg/l	10/9/2020 15:37:52	
PB132247BL	S	Total CN	P	0.5385	µg/l	10/9/2020 15:37:54	
PB132247BS	S	Total CN	P	94.8726	µg/l	10/9/2020 15:37:55	
MIDPB132247	S	Total CN	P	246.6038	µg/l	10/9/2020 15:37:56	
L4214-12	S	Total CN	P	2.8846	µg/l	10/9/2020 15:45:21	
L4327-07	S	Total CN	P	19.0366	µg/l	10/9/2020 15:45:23	
L4327-07DUP	S	Total CN	P	19.1987	µg/l	10/9/2020 15:45:24	
L4327-07MS	S	Total CN	P	53.7175	µg/l	10/9/2020 15:45:25	
L4327-07MSD	S	Total CN	P	53.5506	µg/l	10/9/2020 15:45:26	
CCV2	S	Total CN	P	247.6505	µg/l	10/9/2020 15:45:30	
CCB2	S	Total CN	P	0.4227	µg/l	10/9/2020 15:48:09	