

LB111492

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

10/14/2020 11:01

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.028	0.0	0.109	
ICB1	0.000	0.0	0.004	
CCV1	1.031	0.0	0.110	
CCB1	0.001	0.0	0.005	
PB132326BL	0.002	0.0	0.005	
PB132326BS	1.022	0.0	0.109	
L4214-12	0.026	0.0	0.007	
CCV2	1.037	0.0	0.110	
CCB2	0.002	0.0	0.005	

N	9
Mean	0.461
SD	0.5394
CV%	117.02

Aquakem v. 7.2AQ1

Results from time period:

Wed Oct 14 10:04:35 2020

Wed Oct 14 11:00:06 2020

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0546	mg/l	10/14/2020 10:04:35	
0.1PPM	A	Phenolics-	P	0.1013	mg/l	10/14/2020 10:04:36	
0.25PPM	A	Phenolics-	P	0.2532	mg/l	10/14/2020 10:04:37	
0.50PPM	A	Phenolics-	P	0.4954	mg/l	10/14/2020 10:04:38	
1.0PPM	A	Phenolics-	P	0.9899	mg/l	10/14/2020 10:04:39	
2.0PPM	A	Phenolics-	P	2.0057	mg/l	10/14/2020 10:04:40	
ICV1	S	Phenolics-	P	1.0277	mg/l	10/14/2020 10:30:10	
ICB1	S	Phenolics-	P	0.0005	mg/l	10/14/2020 10:30:12	
CCV1	S	Phenolics-	P	1.0307	mg/l	10/14/2020 10:30:14	
CCB1	S	Phenolics-	P	0.0012	mg/l	10/14/2020 10:30:15	
PB132326BL	S	Phenolics-	P	0.0018	mg/l	10/14/2020 10:30:17	
PB132326BS	S	Phenolics-	P	1.0222	mg/l	10/14/2020 10:30:18	
L4214-12	S	Phenolics-	P	0.0256	mg/l	10/14/2020 11:00:01	
CCV2	S	Phenolics-	P	1.037	mg/l	10/14/2020 11:00:04	
CCB2	S	Phenolics-	P	0.0015	mg/l	10/14/2020 11:00:05	

LB11492

=====

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Am

Instrument ID : Konelab

10/14/2020 10:05

Test Phenolics-


Accepted 10/14/2020 10:05

Factor 9.805

Bias 0.004

Coeff. of det. 0.999932

Errors

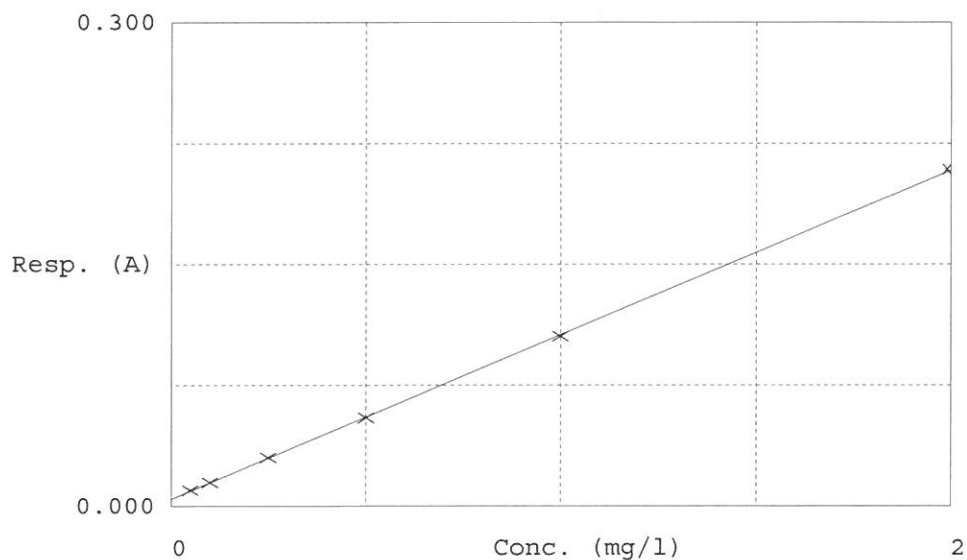

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.010	0.0546	0.0500	
2	Phenol-2	0.015	0.1013	0.1000	
3	Phenol-2	0.030	0.2532	0.2500	
4	Phenol-2	0.055	0.4954	0.5000	
5	Phenol-2	0.105	0.9899	1.0000	
6	Phenol-2	0.209	2.0057	2.0000	