

LB111530

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

10/15/2020 15:18

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.542	0.0	0.083	
ICB1	0.346	0.0	0.001	
CCV1	245.209	0.0	0.213	
CCB1	0.188	0.0	0.000	
PB132360 PB132260BL	0.241	0.0	0.000	
PB132360 PB132260BS	97.007	0.0	0.084	
PB132360 MIDPB132260	244.858	0.0	0.213	
10/15/2020 L4387-07	21.934	0.0	0.019	
AM L4387-07DUP	21.754	0.0	0.019	
L4387-07MS	46.533	0.0	0.041	
L4387-07MSD	46.020	0.0	0.040	
L4386 10/15/2020 CCV2	258.194	0.0	0.224	
AM CCB2	0.369	0.0	0.001	

N	13
Mean	82.938
SD	100.4574
CV%	121.12

Aquakem v. 7.2AQ1

Results from time period:

Thu Oct 15 15:12:57 2020

Thu Oct 15 15:17:19 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.1385	µg/l	10/15/2020 11:31:10	
5.0PPBCN	A	Total CN	P	4.8398	µg/l	10/15/2020 11:31:11	
10PPBCN	A	Total CN	P	9.7556	µg/l	10/15/2020 11:31:12	
50PPBCN	A	Total CN	P	48.7658	µg/l	10/15/2020 11:31:13	
100PPBCN	A	Total CN	P	99.8547	µg/l	10/15/2020 11:31:14	
250PPBCN	A	Total CN	P	252.9732	µg/l	10/15/2020 11:31:15	
500PPBCN	A	Total CN	P	498.6724	µg/l	10/15/2020 11:31:16	
ICV1	S	Total CN	P	95.5423	µg/l	10/15/2020 15:12:57	
ICB1	S	Total CN	P	0.3456	µg/l	10/15/2020 15:12:58	
CCV1	S	Total CN	P	245.2088	µg/l	10/15/2020 15:12:59	
CCB1	S	Total CN	P	0.1884	µg/l	10/15/2020 15:13:00	
PB132360BL	S	Total CN	P	0.2406	µg/l	10/15/2020 15:13:01	
PB132360BS	S	Total CN	P	97.0066	µg/l	10/15/2020 15:13:02	
MIDPB132360	S	Total CN	P	244.8579	µg/l	10/15/2020 15:13:03	
L4386-07	S	Total CN	P	21.9337	µg/l	10/15/2020 15:13:04	
L4386-07DUP	S	Total CN	P	21.7537	µg/l	10/15/2020 15:13:05	
L4386-07MS	S	Total CN	P	46.533	µg/l	10/15/2020 15:13:06	
L4386-07MSD	S	Total CN	P	46.0195	µg/l	10/15/2020 15:13:07	
CCV2	S	Total CN	P	258.1942	µg/l	10/15/2020 15:17:18	
CCB2	S	Total CN	P	0.3694	µg/l	10/15/2020 15:17:19	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

10/15/2020 11:32

Test Total CN


Accepted 10/15/2020 11:31

Factor 1152

Bias 0

Coeff. of det. 0.999940

Errors

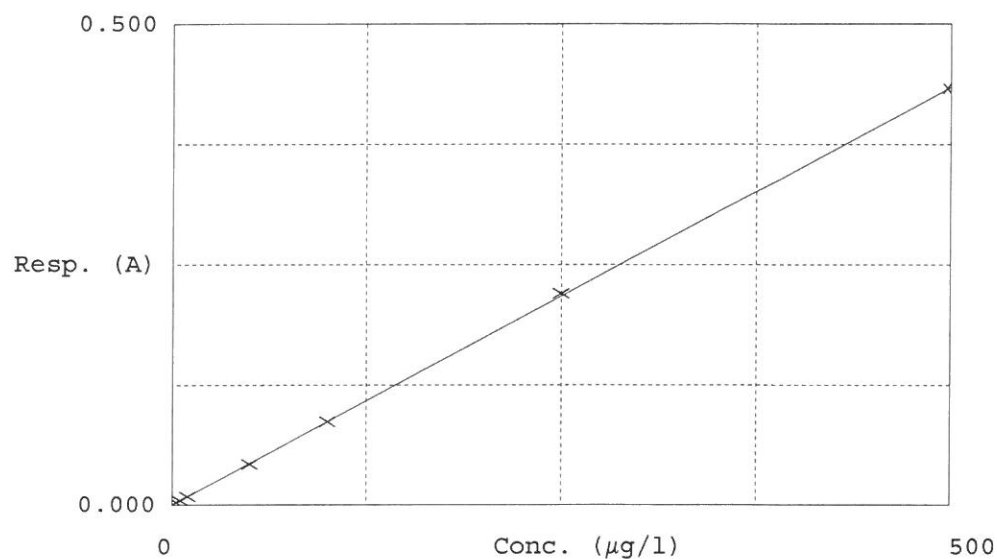

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.1385	0.0000	
2	5.0PPBCN	0.004	4.8398	5.0000	
3	10PPBCN	0.009	9.7556	10.0000	
4	50PPBCN	0.043	48.7658	50.0000	
5	100PPBCN	0.087	99.8547	100.0000	
6	250PPBCN	0.220	252.9732	250.0000	
7	500PPBCN	0.433	498.6724	500.0000	