

LB111624

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

10/21/2020 9:45

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.153	0.0	0.084	
ICB1	0.198	0.0	0.000	
CCV1	248.271	0.0	0.214	
CCB1	0.476	0.0	0.001	
PB132511BL	0.251	0.0	0.001	
PB132511BS	98.537	0.0	0.085	
MIDPB132511	249.036	0.0	0.215	
L4373-01	0.909	0.0	0.001	
L4373-01DUP	0.854	0.0	0.001	
L4373-01MS	29.756	0.0	0.026	
L4373-01MSD	29.914	0.0	0.026	
CCV2	250.208	0.0	0.216	
CCB2	0.394	0.0	0.001	

N	13
Mean	77.381
SD	103.8226
CV%	134.17

Aquakem v. 7.2AQ1

Results from time period:

Wed Oct 21 09:03:22 2020

Wed Oct 21 09:41:56 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.3287	µg/l	10/21/2020 9:03:22	
5.0PPBCN	A	Total CN	P	4.8316	µg/l	10/21/2020 9:03:23	
10PPBCN	A	Total CN	P	10.0897	µg/l	10/21/2020 9:03:24	
50PPBCN	A	Total CN	P	46.5252	µg/l	10/21/2020 9:03:25	
100PPBCN	A	Total CN	P	100.2174	µg/l	10/21/2020 9:03:26	
250PPBCN	A	Total CN	P	255.4068	µg/l	10/21/2020 9:03:27	
500PPBCN	A	Total CN	P	497.6005	µg/l	10/21/2020 9:03:28	
ICV1	S	Total CN	P	97.1529	µg/l	10/21/2020 9:34:12	
ICB1	S	Total CN	P	0.1983	µg/l	10/21/2020 9:34:13	
CCV1	S	Total CN	P	248.2706	µg/l	10/21/2020 9:34:16	
CCB1	S	Total CN	P	0.4755	µg/l	10/21/2020 9:34:17	
PB132511BL	S	Total CN	P	0.2514	µg/l	10/21/2020 9:34:19	
PB132511BS	S	Total CN	P	98.5371	µg/l	10/21/2020 9:34:20	
MIDPB132511	S	Total CN	P	249.0363	µg/l	10/21/2020 9:34:21	
L4373-01	S	Total CN	P	0.9088	µg/l	10/21/2020 9:41:46	
L4373-01DUP	S	Total CN	P	0.8543	µg/l	10/21/2020 9:41:47	
L4373-01MS	S	Total CN	P	29.7559	µg/l	10/21/2020 9:41:50	
L4373-01MSD	S	Total CN	P	29.9145	µg/l	10/21/2020 9:41:51	
CCV2	S	Total CN	P	250.2081	µg/l	10/21/2020 9:41:53	
CCB2	S	Total CN	P	0.3938	µg/l	10/21/2020 9:41:54	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

10/21/2020 9:05


Test Total CN

Accepted 10/21/2020 9:05

Factor 1161
Bias 0

Coeff. of det. 0.999770

Errors

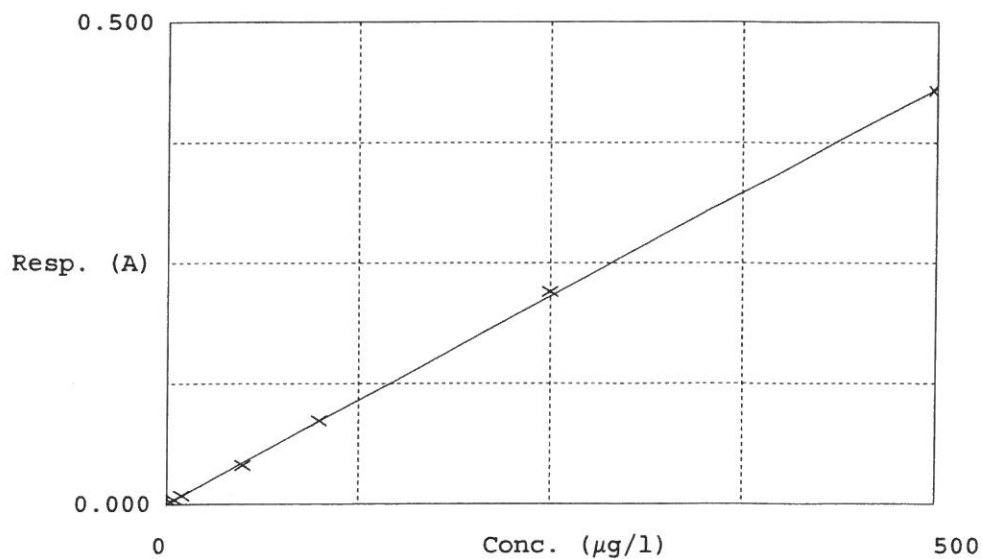

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.3287	0.0000	
2	5.0PPBCN	0.004	4.8316	5.0000	
3	10PPBCN	0.009	10.0897	10.0000	
4	50PPBCN	0.040	46.5252	50.0000	
5	100PPBCN	0.087	100.2174	100.0000	
6	250PPBCN	0.220	255.4068	250.0000	
7	500PPBCN	0.429	497.6005	500.0000	