

LB1M704

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

10/27/2020 13:08

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.762	0.0	0.084	
ICB1	-0.638	0.0	0.001	
CCV1	249.203	0.0	0.214	
CCB1	-0.869	0.0	0.000	
PB132653BL	-0.772	0.0	0.001	
L4219-24	-0.520	0.0	0.001	
L4219-24DUP	-0.725	0.0	0.001	
PB132654BL	-1.210	0.0	0.000	
L4516-02	-1.028	0.0	0.000	
L4516-02DUP	-1.133	0.0	0.000	
L4516-05	-1.158	0.0	0.000	
L4520-02	-0.799	0.0	0.000	
CCV2	257.273	0.0	0.221	
CCB2	-0.519	0.0	0.001	

N	14
Mean	42.419
SD	93.0144
CV%	219.27

Aquakem v. 7.2AQ1

Results from time period:

Tue Oct 27 13:02:21 2020

Tue Oct 27 13:08:10 2020

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	-0.868	µg/l	10/27/2020 9:38:31
5.OPPBCN	A	Reactive CN	P	4.212	µg/l	10/27/2020 9:38:32
10PPBCN	A	Reactive CN	P	9.1668	µg/l	10/27/2020 9:38:33
50PPBCN	A	Reactive CN	P	49.9456	µg/l	10/27/2020 9:38:34
100PPBCN	A	Reactive CN	P	99.6116	µg/l	10/27/2020 9:38:35
250PPBCN	A	Reactive CN	P	255.6486	µg/l	10/27/2020 9:38:36
500PPBCN	A	Reactive CN	P	497.2834	µg/l	10/27/2020 9:38:37
ICV1	S	Reactive CN	P	96.7624	µg/l	10/27/2020 13:02:22
ICB1	S	Reactive CN	P	-0.6385	µg/l	10/27/2020 13:02:23
CCV1	S	Reactive CN	P	249.2028	µg/l	10/27/2020 13:02:26
CCB1	S	Reactive CN	P	-0.869	µg/l	10/27/2020 13:02:27
PB132653BL	S	Reactive CN	P	-0.7722	µg/l	10/27/2020 13:02:29
L4219-24	S	Reactive CN	P	-0.52	µg/l	10/27/2020 13:02:30
L4219-24DUP	S	Reactive CN	P	-0.725	µg/l	10/27/2020 13:02:31
PB132654BL	S	Reactive CN	P	-1.2099	µg/l	10/27/2020 13:08:04
L4516-02	S	Reactive CN	P	-1.0278	µg/l	10/27/2020 13:08:05
L4516-02DUP	S	Reactive CN	P	-1.1328	µg/l	10/27/2020 13:08:06
L4516-05	S	Reactive CN	P	-1.1576	µg/l	10/27/2020 13:08:07
L4520-02	S	Reactive CN	P	-0.799	µg/l	10/27/2020 13:08:08
CCV2	S	Reactive CN	P	257.2732	µg/l	10/27/2020 13:08:09
CCB2	S	Reactive CN	P	-0.5188	µg/l	10/27/2020 13:08:10

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

10/27/2020 9:40


Test Total CN

Accepted 10/27/2020 9:40

Factor 1169
Bias 0.001

Coeff. of det. 0.999798

Errors

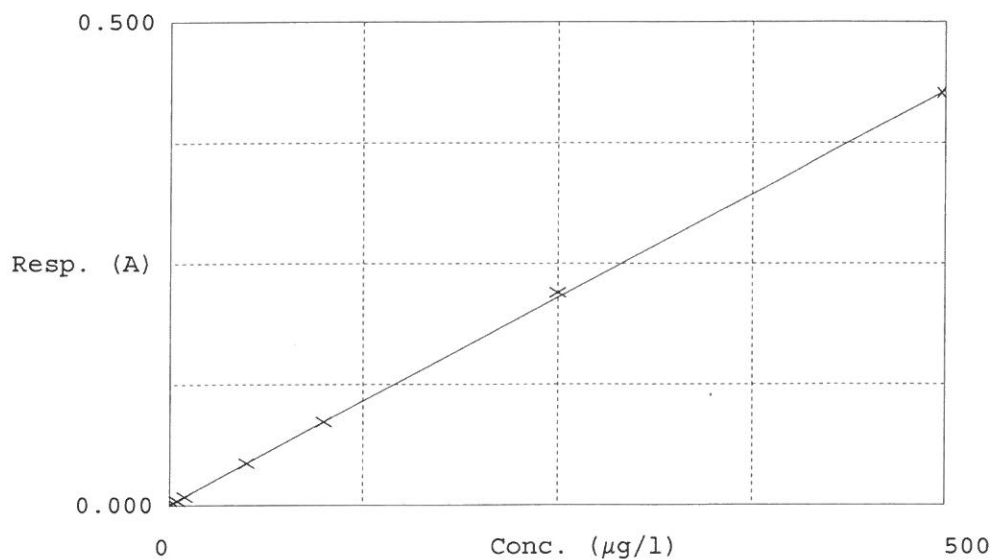

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	-0.8680	0.0000	
2	5.0PPBCN	0.005	4.2120	5.0000	
3	10PPBCN	0.009	9.1668	10.0000	
4	50PPBCN	0.044	49.9456	50.0000	
5	100PPBCN	0.086	99.6116	100.0000	
6	250PPBCN	0.220	255.6486	250.0000	
7	500PPBCN	0.427	497.2834	500.0000	