

IC-1
300-0906A
11/02/2020
AM


Clear table

ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-10-21	10/21/20 9:52		AM/AP
STD2	0.1510	0.3230	0.3550	1.2840	0.2870	0.2070	1.7940	2020-10-21	10/21/20 10:24		AM/AP
STD3	0.4240	0.6210	0.6280	2.1740	0.5530	1.0370	3.2180	2020-10-21	10/21/20 10:55		AM/AP
STD4	0.7410	1.2040	1.2010	4.0050	1.0200	2.2220	6.0340	2020-10-21	10/21/20 11:27		AM/AP
STD5	2.1010	2.9840	2.9670	9.7680	2.4740	5.4800	15.0250	2020-10-21	10/21/20 11:59		AM/AP
STD6	3.9820	6.1310	6.1160	19.8290	5.0570	10.3340	30.7650	2020-10-21	10/21/20 12:31		AM/AP
STD7	4.9840	7.6160	7.6410	25.3730	6.3360	12.4270	37.9110	2020-10-21	10/21/20 13:03		AM/AP
ICV	2.0270	2.9300	2.8810	9.6560	2.3950	5.1140	14.2850	2020-10-21	10/21/20 13:35		AM/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-10-21	10/21/20 14:21		AM/AP
CCV	2.1160	2.8790	2.8710	9.7360	2.3980	4.9490	14.4270	2020-10-29	10/29/20 8:51		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-10-29	10/29/20 9:24		AM/AP
LB111737BLS	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-10-29	10/29/20 9:55	5.00g/100mL	AM/AP
LB111737BSS	2.1170	2.8250	2.9630	9.8950	2.3930	5.1980	14.8800	2020-10-29	10/29/20 10:49	5.00g/100mL	AM/AP
L4548-01	2.5770	40.2230	0.0000	2.6420	23.3080	4.8340	41.7430	2020-10-29	10/29/20 12:02	5.02g/100mL	AM/AP
L4214-01	0.1130	0.2160	0.2760	0.8270	0.1810	0.1330	1.1690	2020-10-29	10/29/20 13:06	5.00g/100mL	AM/AP
L4214-02	0.2330	0.3450	0.3950	1.2340	0.2970	0.3410	1.8250	2020-10-29	10/29/20 14:10	5.00g/100mL	AM/AP
L4214-02RE	0.3260	0.6150	0.6710	2.1750	0.5250	0.7230	3.1770	2020-10-29	10/29/20 14:42	5.00g/100mL	AM/AP
L4548-01DLX2	0.9880	18.3820	0.0000	1.5180	10.7210	2.1530	19.5990	2020-10-29	10/29/20 15:14	5.02g/100mL	AM/AP
L4548-01DL2X10	0.2540	3.3240	0.0000	0.5800	2.0040	0.6780	4.1910	2020-10-29	10/29/20 15:49	5.02g/100mL	AM/AP
CCV	2.1200	2.9410	2.8810	9.8260	2.4290	5.2520	14.9330	2020-10-29	10/29/20 16:21		AM/AP
CCB								2020-10-29	10/29/20 17:05		AM/AP

CALIBRATION OF COMPONENT F-

IC-1
300.0
10/21/2020
AM

Method: ANIONS 10-21-20.mtw
Equation: $Q = 0.918264 \cdot A + 0.765631$
RSD: 3.031 %
Correlation coefficient: 0.999612

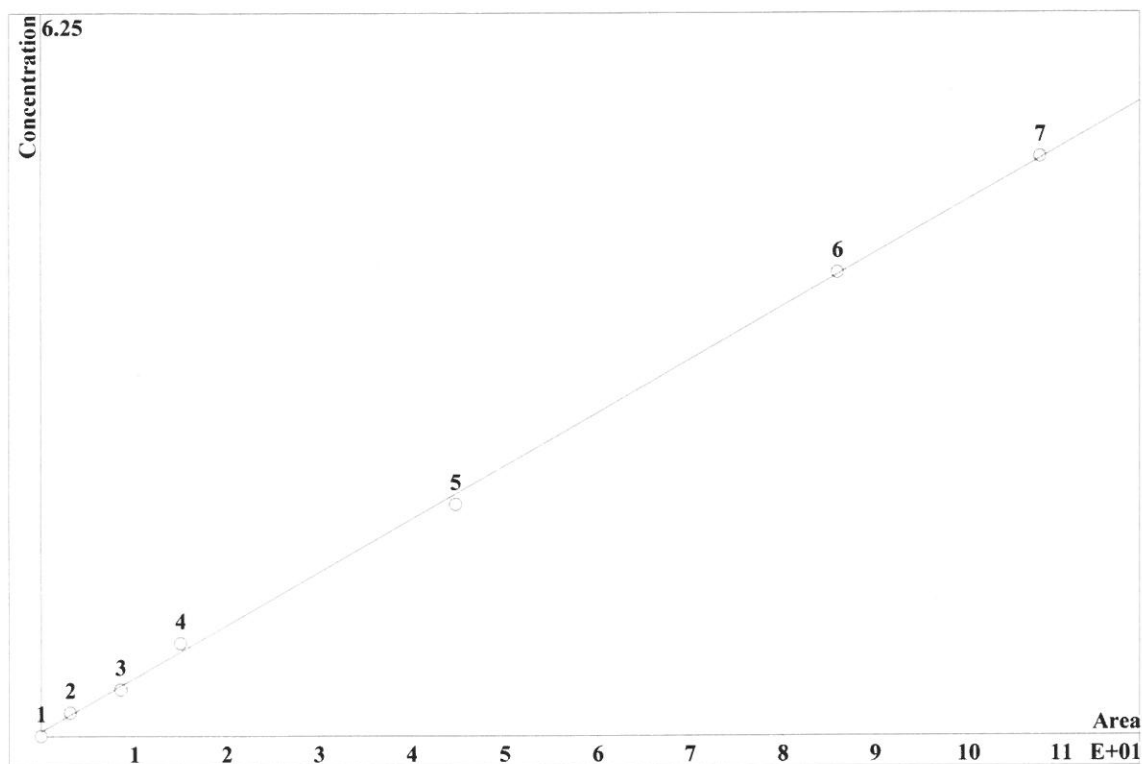

K3 = 0 K2 = 0 K1 = 0.918264 K0 = 0.765631

Base: Area

Ref.channel: Cond

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.1601	3.153	0.2	20	5.718			Yes
3	0.3213	8.596	0.4	20	5.718			Yes
4	0.6734	14.98	0.8	20	5.718			Yes
5	1.956	44.71	2	20	5.718			Yes
6	4.097	85.91	4	20	5.718			Yes
7	5.106	107.7	5	20	5.718			Yes

CALIBRATION OF COMPONENT CL-

Method: ANIONS 10-21-20.mtw
 Equation: $Q = 1.39326 \cdot A + 1.50457$
 RSD: 3.440 %
 Correlation coefficient: 0.999500

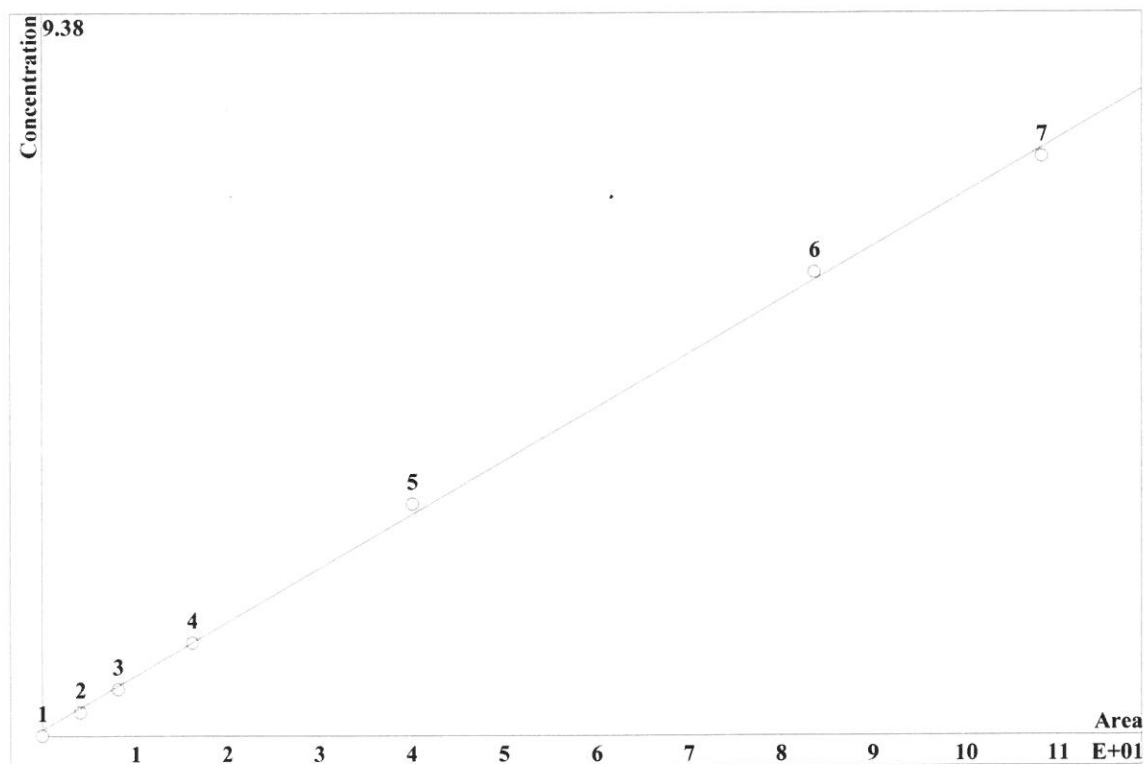

K3 = 0 K2 = 0 K1 = 1.39326 K0 = 1.50457

Base: Area

Ref.channel: Cond

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.2646	4.081	0.3	20	8.798			Yes
3	0.5382	8.181	0.6	20	8.798			Yes
4	1.059	16.23	1.2	20	8.798			Yes
5	2.687	40.11	3	20	8.798			Yes
6	5.722	83.67	6	20	8.798			Yes
7	7.384	108.2	7.5	20	8.798			Yes

CALIBRATION OF COMPONENT
NO2

Method: ANIONS 10-21-20.mtw
Equation: $Q = 0.599456 \cdot A + 2.8051$
RSD: 4.284 %
Correlation coefficient: 0.999224

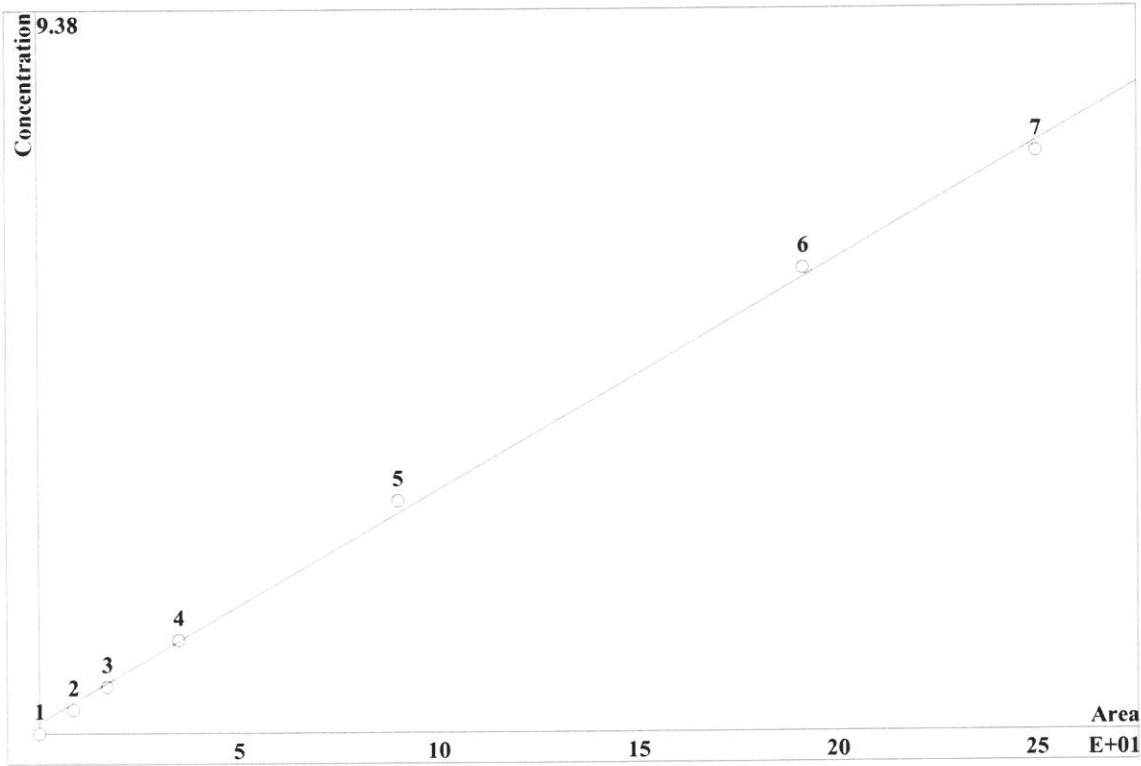


K3 = 0 K2 = 0 K1 = 0.599456 K0 = 2.8051
Base: Area
Ref.channel: Cond
ISTD:
Formula: Linear
Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0		0	No
2	0.4521	8.493	0.3	20	10.57			Yes
3	0.9262	17.06	0.6	20	10.57			Yes
4	1.892	34.98	1.2	20	10.57			Yes
5	4.821	90.05	3	20	10.57			Yes
6	9.957	191.7	6	20	10.57			Yes
7	12.59	250.2	7.5	20	10.57			Yes

CALIBRATION OF COMPONENT BR-

Method: ANIONS 10-21-20.mtw
 Equation: $Q = 3.21197 \cdot A + 7.27565$
 RSD: 3.349 %
 Correlation coefficient: 0.999526

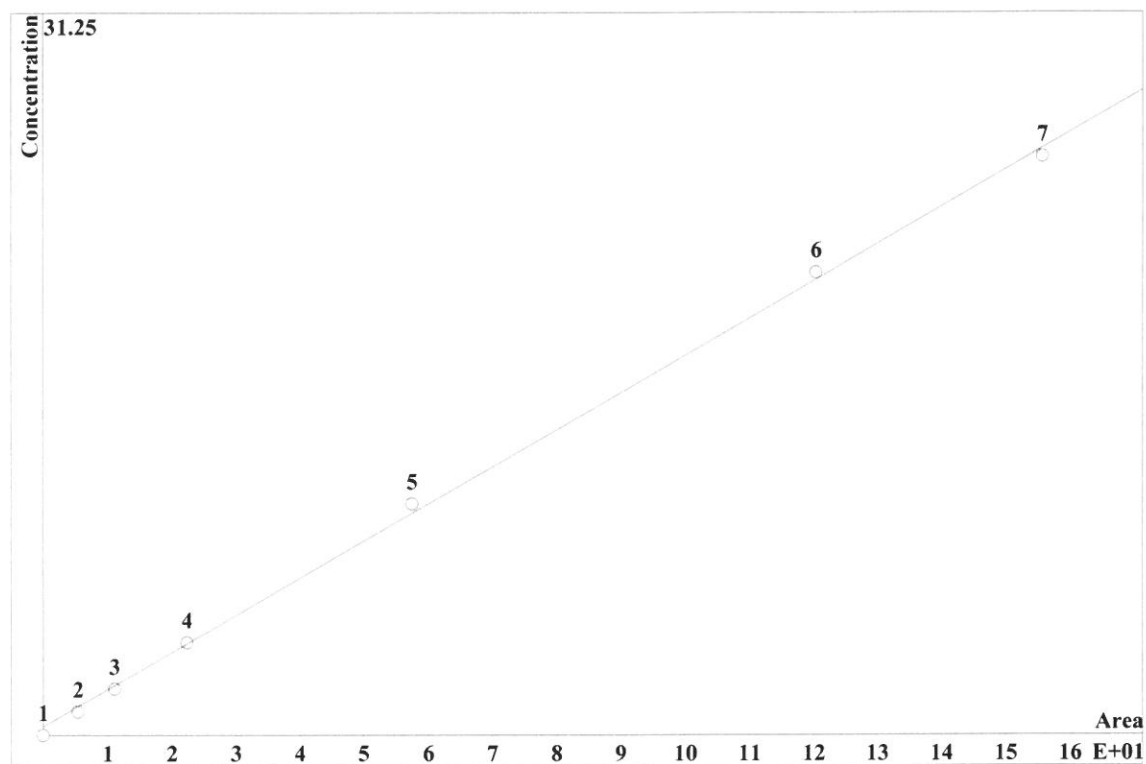

K3 = 0 K2 = 0 K1 = 3.21197 K0 = 7.27565

Base: Area

Ref.channel: Cond

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.2296	5.45	1	20	13.6	Yes		Yes
3	0.4785	11.11	2	20	13.6	Yes		Yes
4	0.9866	22.33	4	20	13.6	Yes		Yes
5	2.588	57.47	10	20	13.6	Yes		Yes
6	5.519	120.4	20	20	13.6	Yes		Yes
7	7.168	155.7	25	20	13.6	Yes		Yes

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	0	No
2	0.2729	8.015	0.25	20	15.54	Yes	
3	0.6046	17.62	0.5	20	15.54	Yes	
4	1.184	33.79	1	20	15.54	Yes	
5	3.003	82.5	2.5	20	15.54	Yes	
6	6.303	171.5	5	20	15.54	Yes	
7	8.206	220.8	6.25	20	15.54	Yes	

CALIBRATION OF COMPONENT HPO4

Method: ANIONS 10-21-20.mtw
 Equation: $Q = 1.33739 \cdot A - 5.3391$
 RSD: 3.688 %
 Correlation coefficient: 0.999425

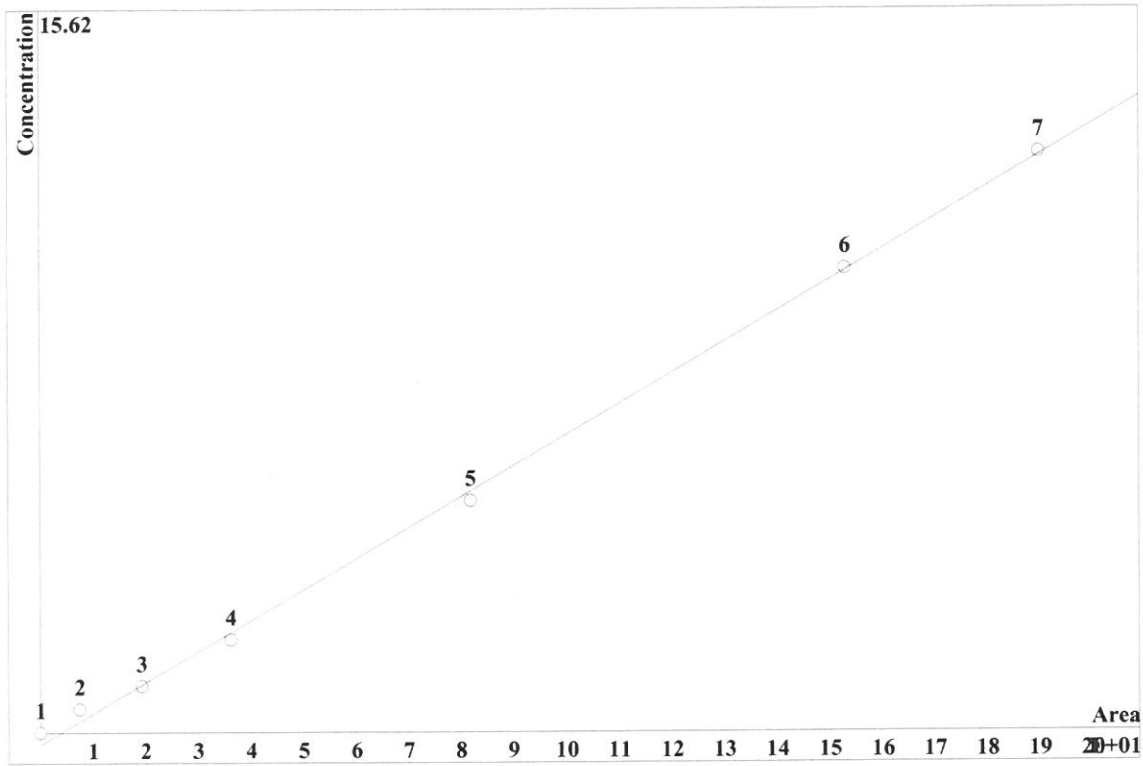


K3 = 0 K2 = 0 K1 = 1.33739 K0 = -5.3391
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.1611	7.495	0.5	20	21.75			Yes
3	0.41	19.31	1	20	21.75			Yes
4	0.8275	36.22	2	20	21.75			Yes
5	1.949	81.85	5	20	21.75			Yes
6	3.747	152.8	10	20	21.75			Yes
7	4.71	189.8	12.5	20	21.75			Yes

CALIBRATION OF COMPONENT SO4

Method: ANIONS 10-21-20.mtw
 Equation: $Q = 1.8684 \cdot A + 7.87171$
 RSD: 2.868 %
 Correlation coefficient: 0.999652

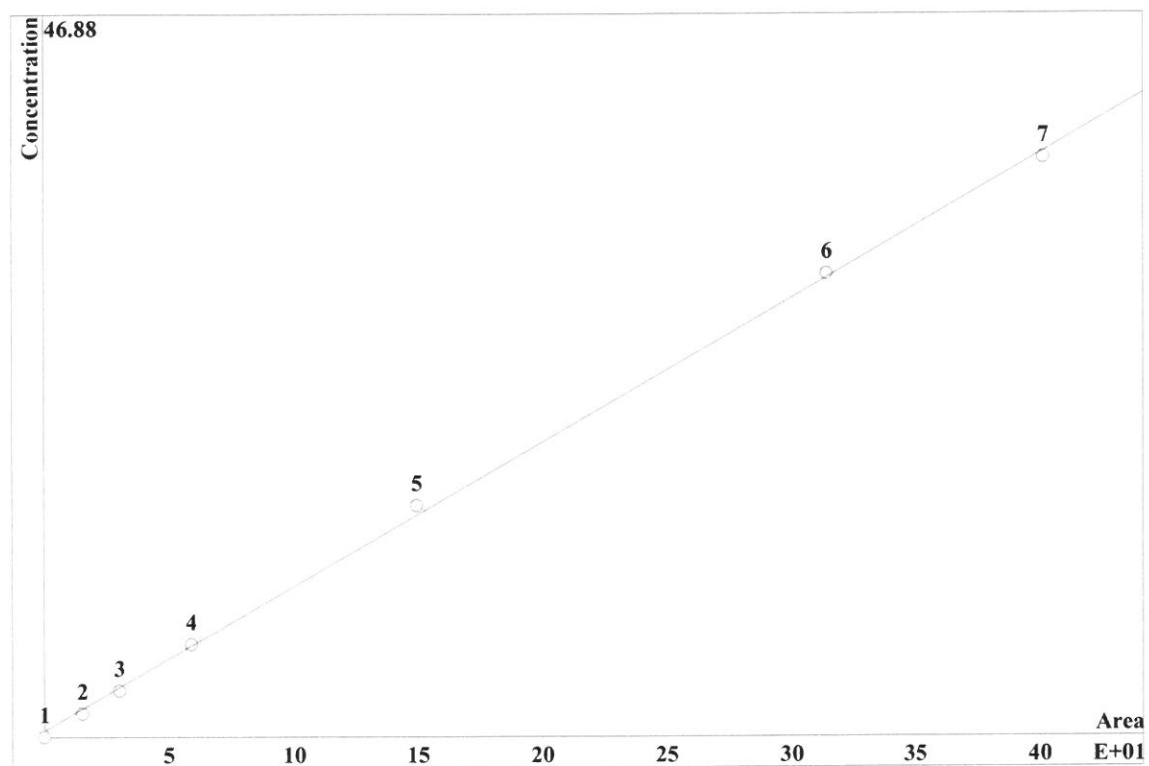

K3 = 0 K2 = 0 K1 = 1.8684 K0 = 7.87171

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0		0	No
2	0.3746	15.35	1.5	20	25.43			Yes
3	0.7421	30.36	3	20	25.43			Yes
4	1.489	58.99	6	20	25.43			Yes
5	3.819	149.7	15	20	25.43			Yes
6	8.032	314.3	30	20	25.43			Yes
7	10.39	401.6	37.5	20	25.43			Yes

Report date: 10/21/2020 1:44:14 PM
Printed by: wet


Ident: STD1
Analysis from: 10/21/2020 9:52:10 AM
File: _2020-10-21_

Last save: 10/21/2020 10:20:58 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 71947

Last save: 10/21/2020 9:42:32 AM

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

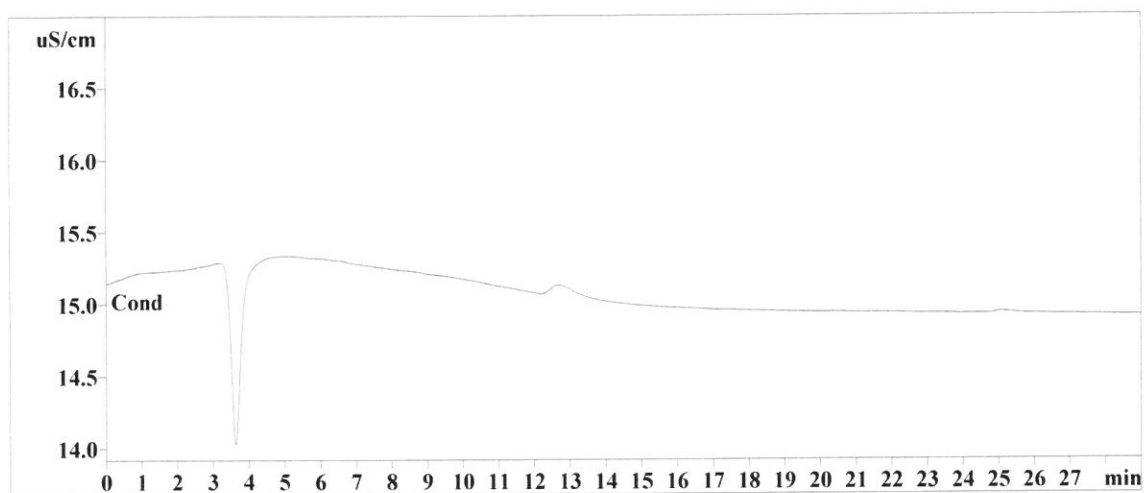

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/21/2020 1:44:20 PM
Printed by: wet


Ident: STD2
Analysis from: 10/21/2020 10:24:04 AM
File: _2020-10-21_

Last save: 10/21/2020 10:52:52 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 71948

Last save: 10/21/2020 10:20:58 AM

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

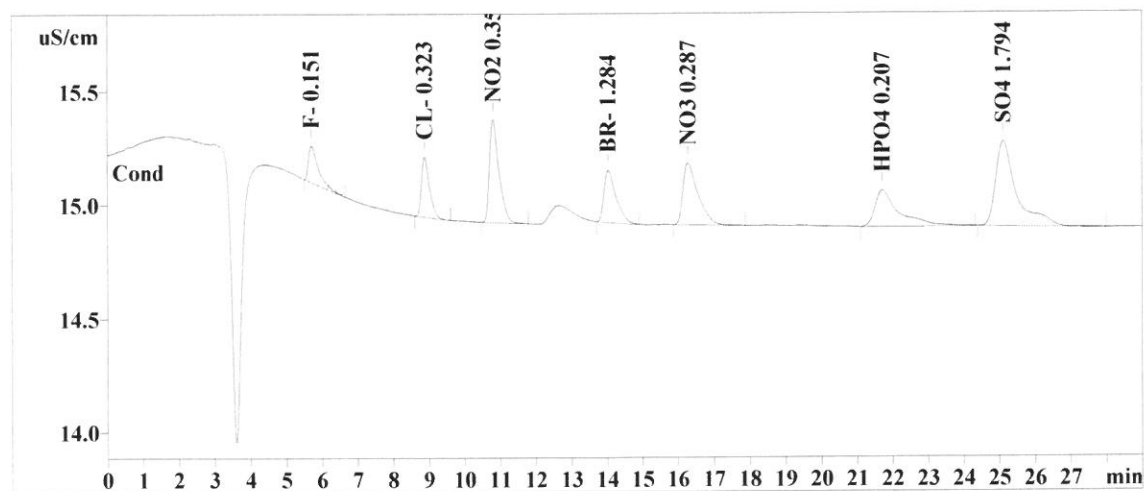

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.271	0.16	8.36	3.153	6.06	0.
2	8.88	0.227	0.26	13.81	4.081	7.84	0.
3	10.80	0.275	0.45	23.62	8.493	16.32	0.
4	14.03	0.351	0.23	11.95	5.450	10.47	0.
5	16.28	0.433	0.27	14.22	8.015	15.40	0.
6	21.71	0.552	0.16	8.40	7.495	14.40	0.
7	25.11	0.517	0.37	19.54	15.351	29.50	0.
7	29.00	0.375	1.91	99.89	52.038	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 10/21/2020 1:44:25 PM
Printed by: wet


Ident: STD3
Analysis from: 10/21/2020 10:55:58 AM
File: _2020-10-21_

Last save: 10/21/2020 11:24:46 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 71949

Last save: 10/21/2020 10:52:52 AM

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

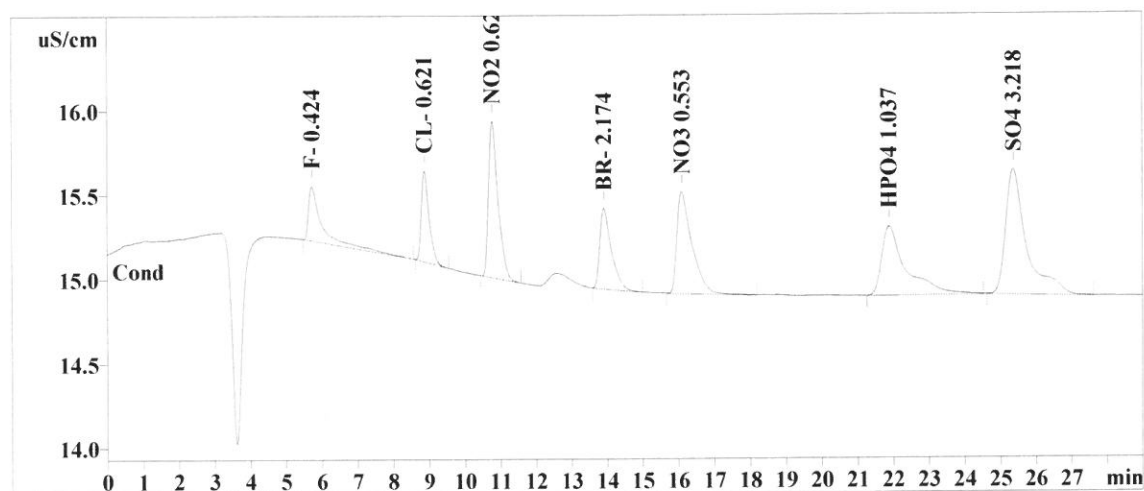

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.280	0.32	7.98	8.596	7.66	0.
2	8.86	0.224	0.54	13.38	8.181	7.29	0.
3	10.77	0.272	0.93	23.02	17.058	15.20	0.
4	13.90	0.340	0.48	11.87	11.112	9.90	0.
5	16.09	0.425	0.60	15.03	17.620	15.70	0.
6	21.88	0.549	0.41	10.20	19.308	17.20	0.
7	25.37	0.522	0.74	18.45	30.363	27.05	0.
7	29.00	0.373	4.02	99.94	112.238	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 10/21/2020 1:44:31 PM
Printed by: wet


Ident: STD4
Analysis from: 10/21/2020 11:27:53 AM
File: _2020-10-21_

Last save: 10/21/2020 11:56:42 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 71950

Last save: 10/21/2020 11:24:46 AM

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

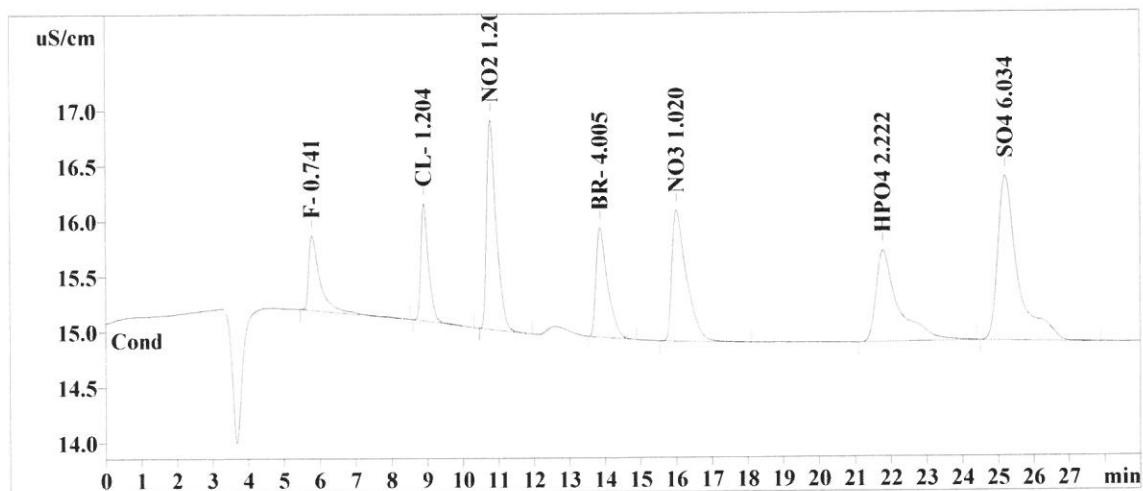

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.79	0.281	0.67	8.29	14.980	6.89	0.
2	8.90	0.221	1.06	13.05	16.234	7.46	0.
3	10.77	0.273	1.89	23.32	34.976	16.08	0.
4	13.86	0.331	0.99	12.16	22.331	10.27	0.
5	16.00	0.418	1.18	14.60	33.792	15.54	0.
6	21.78	0.524	0.83	10.20	36.221	16.65	0.
7	25.20	0.505	1.49	18.35	58.987	27.12	0.
7	29.00	0.365	8.11	99.97	217.521	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 10/21/2020 1:44:36 PM
Printed by: wet


Ident: STD5
Analysis from: 10/21/2020 11:59:47 AM
File: _2020-10-21_

Last save: 10/21/2020 12:28:36 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 71951

Last save: 10/21/2020 11:56:42 AM

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

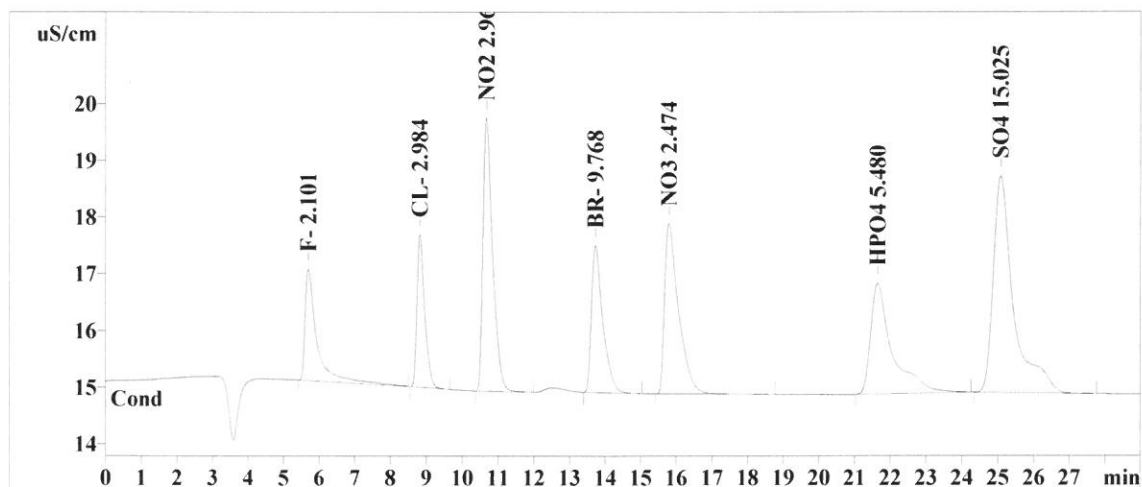

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.70	0.270	1.96	9.39	44.712	8.18	0.
2	8.82	0.219	2.69	12.90	40.105	7.34	0.
3	10.67	0.278	4.82	23.15	90.046	16.48	0.
4	13.72	0.322	2.59	12.43	57.468	10.52	0.
5	15.79	0.403	3.00	14.42	82.499	15.10	0.
6	21.65	0.508	1.95	9.36	81.846	14.98	0.
7	25.08	0.504	3.82	18.34	149.663	27.39	0.
7	29.00	0.358	20.82	99.99	546.339	100.00	0.


This report has been created by IC Net
METROHM LTD

Report date: 10/21/2020 1:44:42 PM
Printed by: wet

Ident: STD6
Analysis from: 10/21/2020 12:31:41 PM
File: _2020-10-21_ Last save: 10/21/2020 1:00:30 PM

Method: ANIONS 10-21-20.mtw Last save: 10/21/2020 12:28:36 PM
Run operator: wet
Analysis number: 71952

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

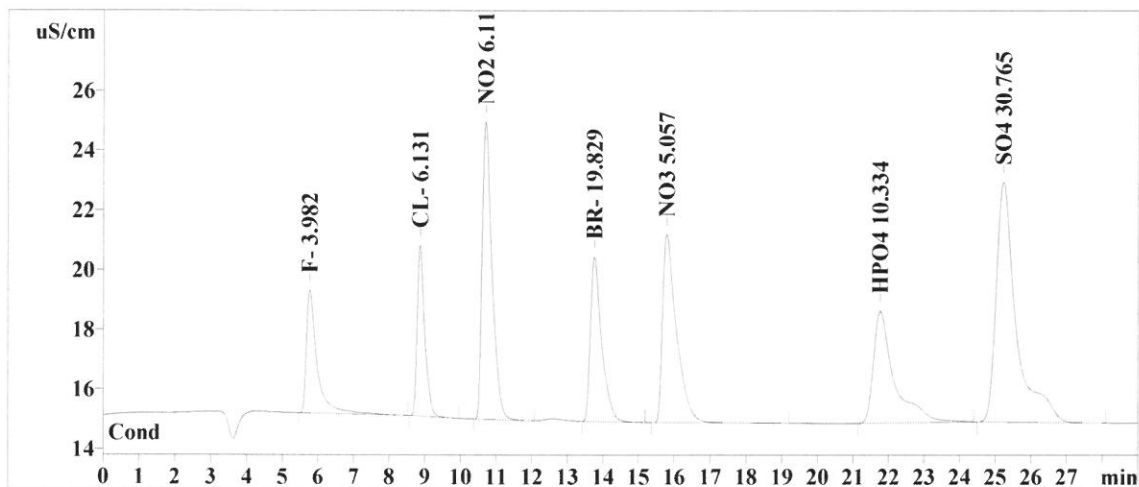

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.76	0.267	4.10	9.44	85.906	7.67	0.
2	8.86	0.212	5.72	13.19	83.670	7.47	0.
3	10.70	0.288	9.96	22.96	191.675	17.11	0.
4	13.75	0.314	5.52	12.72	120.376	10.75	0.
5	15.78	0.399	6.30	14.53	171.462	15.31	0.
6	21.76	0.500	3.75	8.64	152.838	13.64	0.
7	25.22	0.504	8.03	18.52	314.262	28.05	0.
7	29.00	0.355	43.37	99.99	1120.189	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 10/21/2020 1:44:48 PM
 Printed by: wet


Ident: STD7
 Analysis from: 10/21/2020 1:03:35 PM
 File: _2020-10-21_

Last save: 10/21/2020 1:32:24 PM

Method: ANIONS 10-21-20.mtw
 Run operator: wet
 Analysis number: 71953

Last save: 10/21/2020 1:00:30 PM

SAMPLE:
 : AM/AP
 Vial number: 8
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

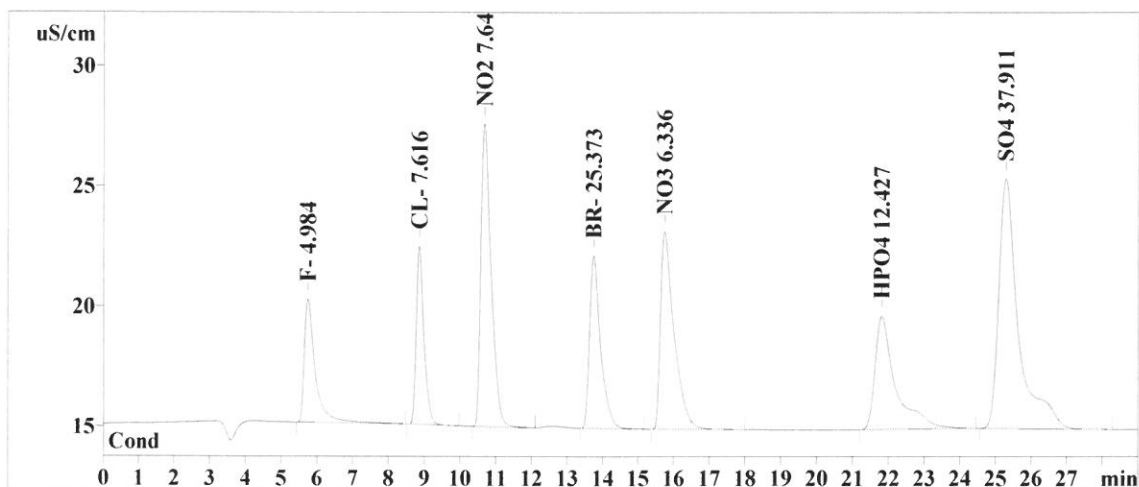

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.74	0.277	5.11	9.19	107.725	7.51	0.
2	8.85	0.213	7.38	13.29	108.249	7.55	0.
3	10.67	0.302	12.59	22.66	250.238	17.45	0.
4	13.74	0.312	7.17	12.90	155.727	10.86	0.
5	15.73	0.395	8.20	14.77	220.791	15.40	0.
6	21.80	0.495	4.71	8.48	189.836	13.24	0.
7	25.28	0.497	10.39	18.70	401.603	28.00	0.
7	29.00	0.356	55.55	100.00	1434.168	100.00	0.

This report has been created by IC Net
 METROHM LTD

Report date: 10/21/2020 3:45:13 PM
Printed by: wet


Ident: ICV
Analysis from: 10/21/2020 1:35:29 PM
File: _2020-10-21_

Last save: 10/21/2020 2:04:18 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 71954

Last save: 10/21/2020 1:32:24 PM

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

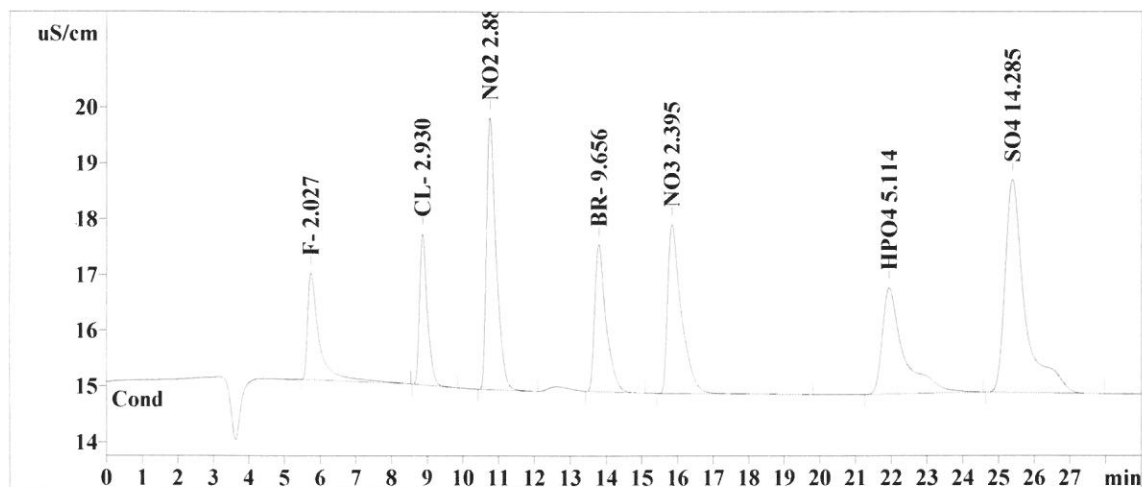

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.74	0.274	1.91	9.16	43.317	7.95	0.
2	8.86	0.221	2.70	12.93	40.982	7.52	0.
3	10.76	0.278	4.87	23.33	91.454	16.77	0.
4	13.78	0.315	2.64	12.64	57.860	10.61	0.
5	15.83	0.392	3.03	14.51	82.430	15.12	0.
6	21.94	0.508	1.90	9.12	80.470	14.76	0.
7	25.39	0.500	3.82	18.29	148.697	27.27	0.
7	29.00	0.355	20.87	99.99	545.210	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 10/21/2020 3:45:20 PM
Printed by: wet


Ident: ICB
Analysis from: 10/21/2020 2:21:03 PM
File: _2020-10-21_

Last save: 10/21/2020 2:49:52 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 71955

Last save: 10/21/2020 1:32:24 PM

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

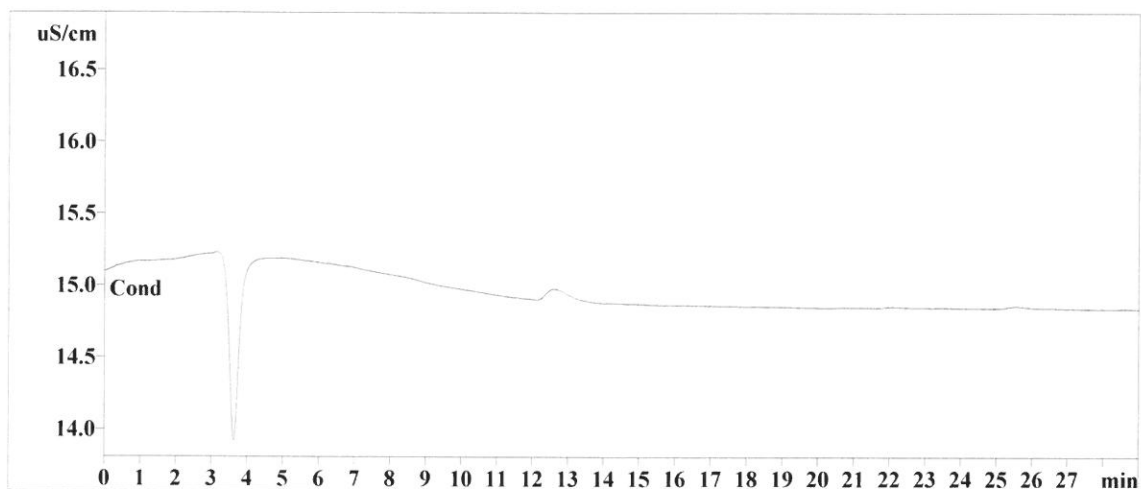

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:43:06 PM
Printed by: wet


Ident: CCV
Analysis from: 10/29/2020 8:51:02 AM
File: _2020-10-29_

Last save: 10/29/2020 9:19:50 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72065

Last save: 10/23/2020 12:59:28 PM

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

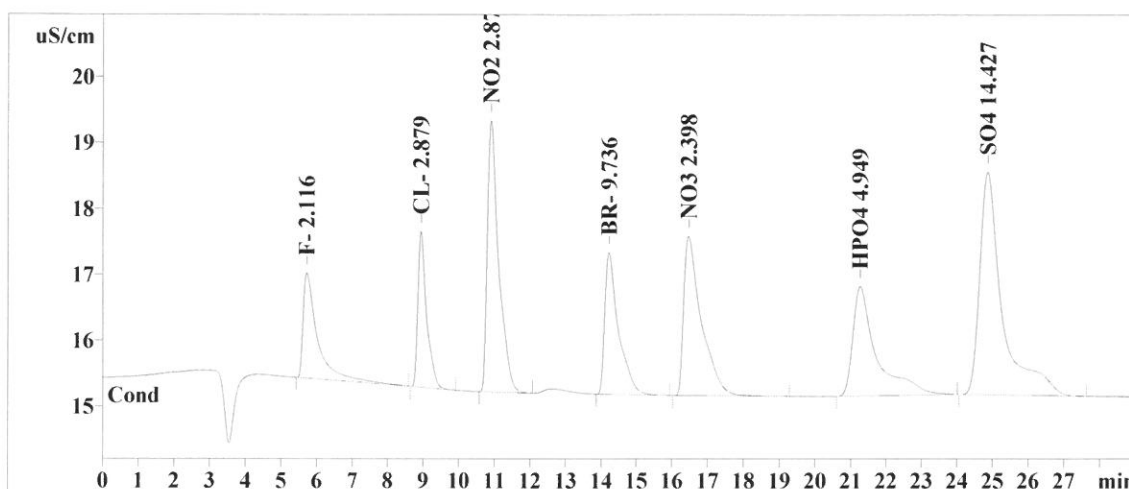

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.350	1.59	9.02	45.245	8.29	0.
2	8.93	0.236	2.36	13.35	40.248	7.38	0.
3	10.89	0.313	4.12	23.30	91.116	16.70	0.
4	14.21	0.371	2.15	12.16	58.361	10.69	0.
5	16.45	0.473	2.41	13.64	82.518	15.12	0.
6	21.26	0.555	1.66	9.40	78.003	14.29	0.
7	24.85	0.550	3.38	19.12	150.215	27.53	0.
7	29.00	0.407	17.67	99.99	545.705	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:43:13 PM
Printed by: wet


Ident: CCB
Analysis from: 10/29/2020 9:24:03 AM
File: _2020-10-29_

Last save: 10/29/2020 9:52:52 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72066

Last save: 10/23/2020 12:59:28 PM

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

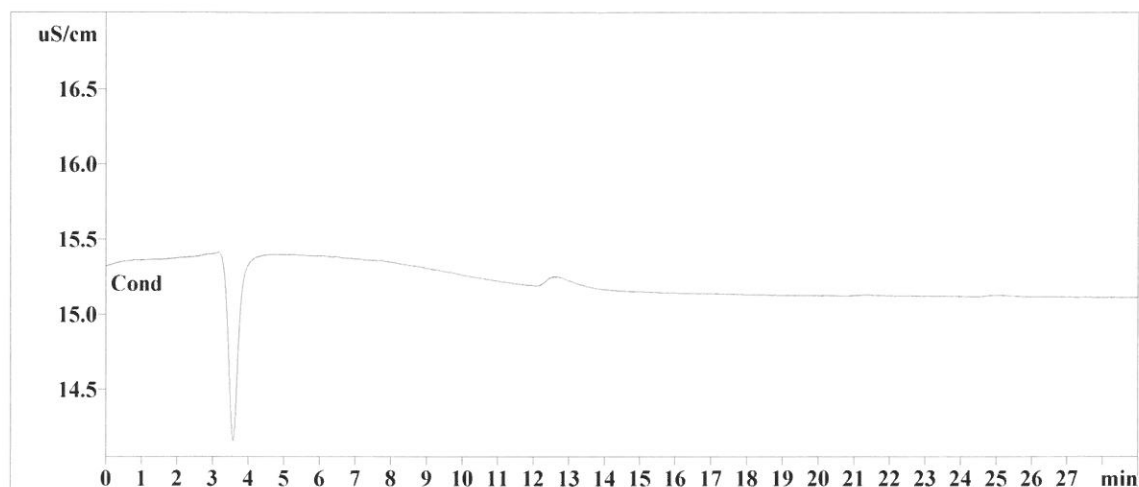

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:43:20 PM
Printed by: wet


Ident: LB111737BLS
Analysis from: 10/29/2020 9:55:58 AM
File: _2020-10-29_

Last save: 10/29/2020 10:24:46 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72067

Last save: 10/23/2020 12:59:28 PM

SAMPLE: 5.00g/100mL
: AM/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

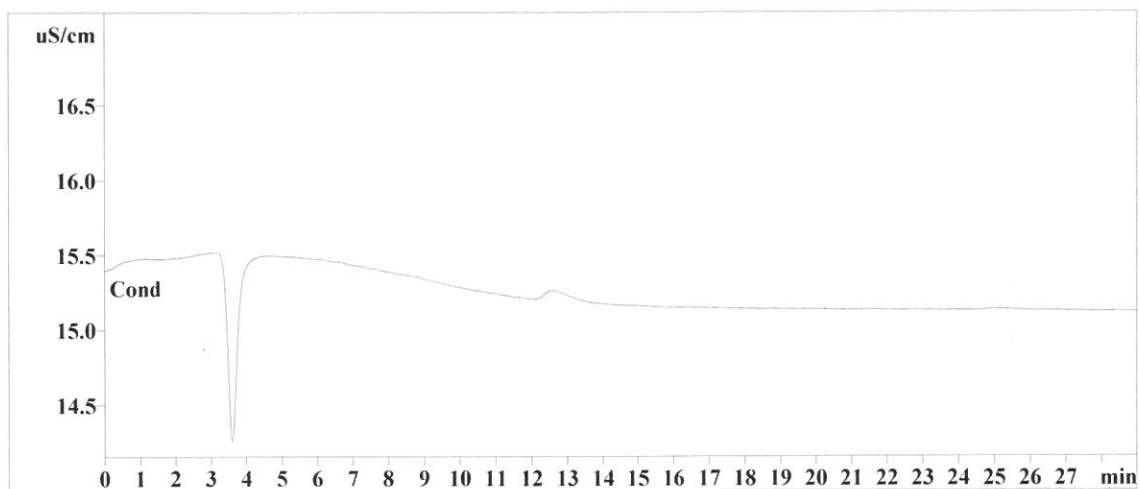

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:43:27 PM
Printed by: wet


Ident: LB111737BSS
Analysis from: 10/29/2020 10:49:46 AM
File: _2020-10-29_

Last save: 10/29/2020 11:18:34 AM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72070

Last save: 10/23/2020 12:59:28 PM

SAMPLE: 5.00g/100mL
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

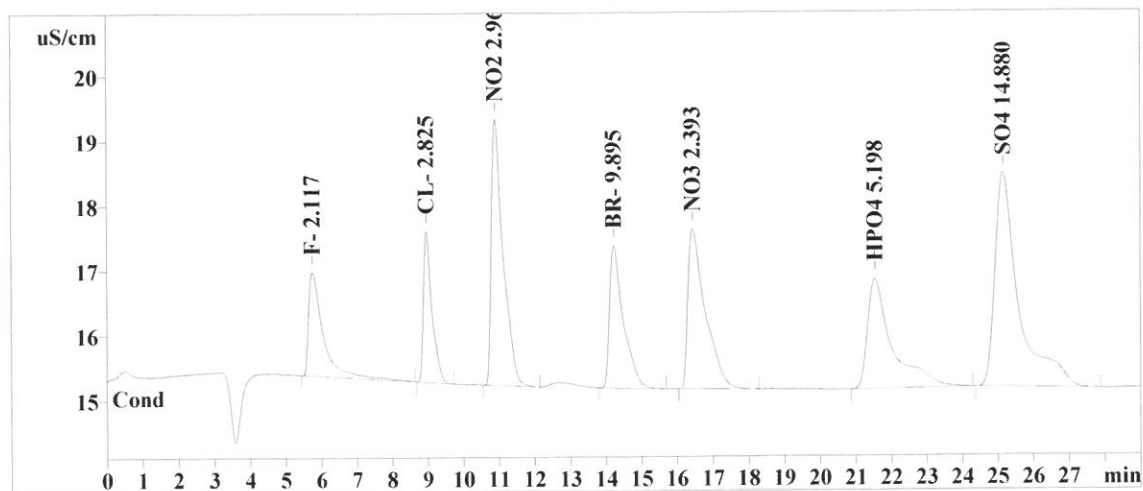

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.75	0.356	1.59	9.02	45.271	8.12	0.
2	8.96	0.241	2.32	13.15	39.478	7.08	0.
3	10.90	0.330	4.10	23.23	94.182	16.90	0.
4	14.22	0.377	2.19	12.40	59.347	10.65	0.
5	16.44	0.475	2.46	13.94	82.344	14.77	0.
6	21.54	0.569	1.69	9.59	81.720	14.66	0.
7	25.15	0.588	3.30	18.66	155.072	27.82	0.
7	29.00	0.419	17.66	99.98	557.413	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:43:35 PM
 Printed by: wet


Ident: L4548-01
 Analysis from: 10/29/2020 12:02:44 PM
 File: _2020-10-29_

Last save: 11/2/2020 1:36:58 PM

Method: ANIONS 10-21-20.mtw
 Run operator: wet
 Analysis number: 72071

Last save: 10/23/2020 12:59:28 PM

SAMPLE: 5.02g/100mL
 : AM/AP
 Vial number: 9
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

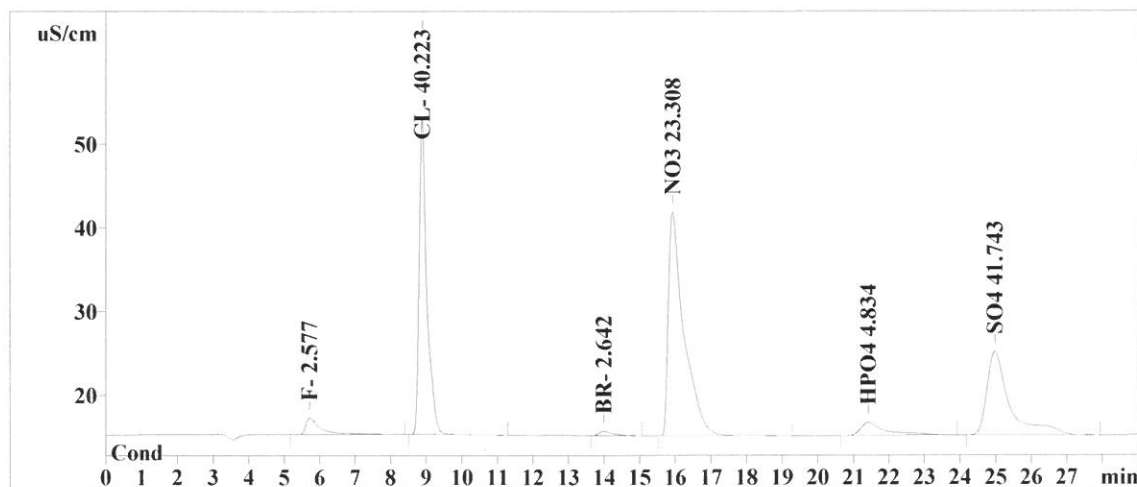

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.356	1.91	2.44	55.297	2.79	0.
2	8.88	0.206	37.84	48.23	576.313	29.09	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	13.99	0.379	0.53	0.67	14.185	0.72	0.
5	15.91	0.414	26.68	34.00	816.765	41.22	0.
6	21.41	0.583	1.54	1.96	76.278	3.85	0.
7	24.97	0.549	9.95	12.69	442.616	22.34	0.
7	29.00	0.355	78.45	100.00	1981.454	100.00	0.

This report has been created by IC Net
 METROHM LTD

Report date: 11/2/2020 1:43:42 PM

Printed by: wet

Ident: L4214-01

Analysis from: 10/29/2020 1:06:32 PM

File: _2020-10-29_

Last save: 10/29/2020 1:45:00 PM

Method: ANIONS 10-21-20.mtw

Last save: 10/23/2020 12:59:28 PM

Run operator: wet

Analysis number: 72073

SAMPLE: 5.00g/100mL


: AM/AP

Vial number: 6

Volume: 20.0 µL

Dilution: 1.00

Amount: 1.0000

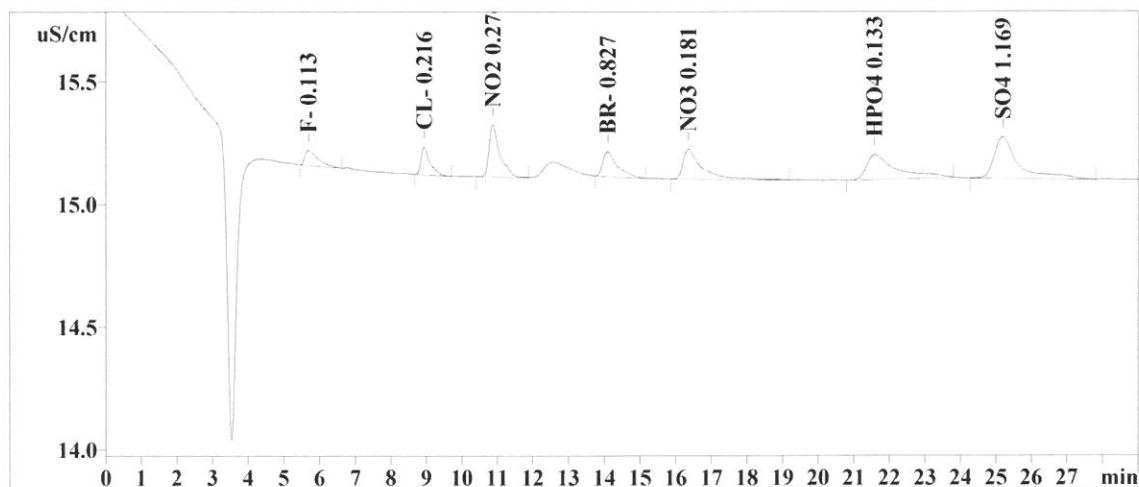

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.69	0.373	0.06	7.03	1.623	5.41	0.
2	8.93	0.239	0.11	12.71	2.024	6.75	0.
3	10.87	0.286	0.21	23.81	4.524	15.09	0.
4	14.08	0.379	0.10	11.43	2.884	9.62	0.
5	16.35	0.442	0.12	13.81	4.656	15.53	0.
6	21.59	0.717	0.10	11.50	5.975	19.93	0.
7	25.18	0.585	0.17	19.21	8.296	27.67	0.
7	29.00	0.432	0.88	99.49	29.982	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:43:50 PM
Printed by: wet


Ident: L4214-02
Analysis from: 10/29/2020 2:10:20 PM
File: _2020-10-29_

Last save: 10/29/2020 2:39:08 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72075

Last save: 10/23/2020 12:59:28 PM

SAMPLE: 5.00g/100mL
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

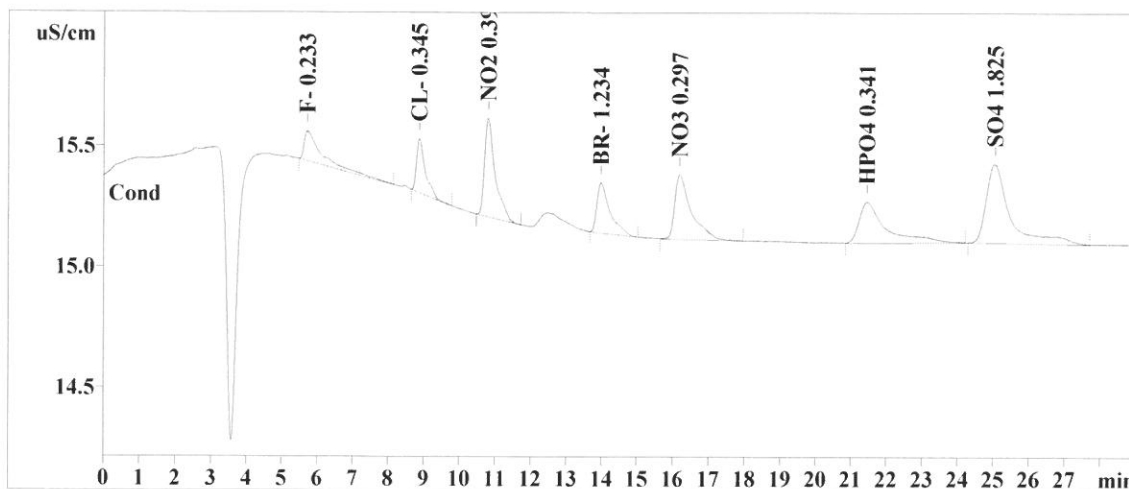

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.370	0.12	7.13	4.247	7.69	0.
2	8.86	0.231	0.22	12.90	3.866	7.00	0.
3	10.79	0.282	0.41	23.54	8.498	15.39	0.
4	13.97	0.350	0.21	12.02	5.418	9.81	0.
5	16.19	0.425	0.27	15.50	8.761	15.87	0.
6	21.45	0.618	0.17	9.85	9.094	16.47	0.
7	25.03	0.573	0.33	18.91	15.323	27.76	0.
7	29.00	0.407	1.73	99.84	55.207	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:43:58 PM
Printed by: wet


Ident: L4214-02RE
Analysis from: 10/29/2020 2:42:14 PM
File: _2020-10-29_

Last save: 10/29/2020 3:11:02 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72076

Last save: 10/23/2020 12:59:28 PM

SAMPLE: 5.00g/100mL
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

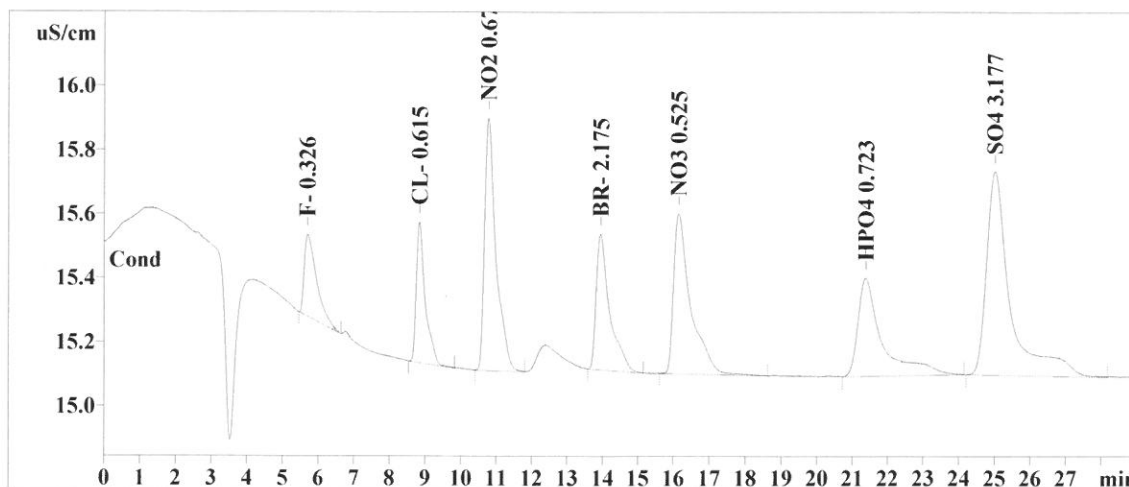

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.70	0.358	0.26	7.62	6.265	6.00	0.
2	8.83	0.238	0.44	13.08	7.744	7.42	0.
3	10.77	0.310	0.79	23.53	17.724	16.99	0.
4	13.93	0.351	0.42	12.63	11.279	10.81	0.
5	16.14	0.432	0.50	14.95	16.736	16.04	0.
6	21.37	0.564	0.31	9.14	14.804	14.19	0.
7	25.00	0.570	0.64	18.95	29.794	28.55	0.
7	29.00	0.403	3.35	99.89	104.346	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:44:15 PM
Printed by: wet


Ident: L4548-01DLX2
Analysis from: 10/29/2020 3:14:08 PM
File: _2020-10-29_

Last save: 10/29/2020 3:42:56 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72077

Last save: 10/23/2020 12:59:28 PM

SAMPLE: 5.02g/100mL
: AM/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

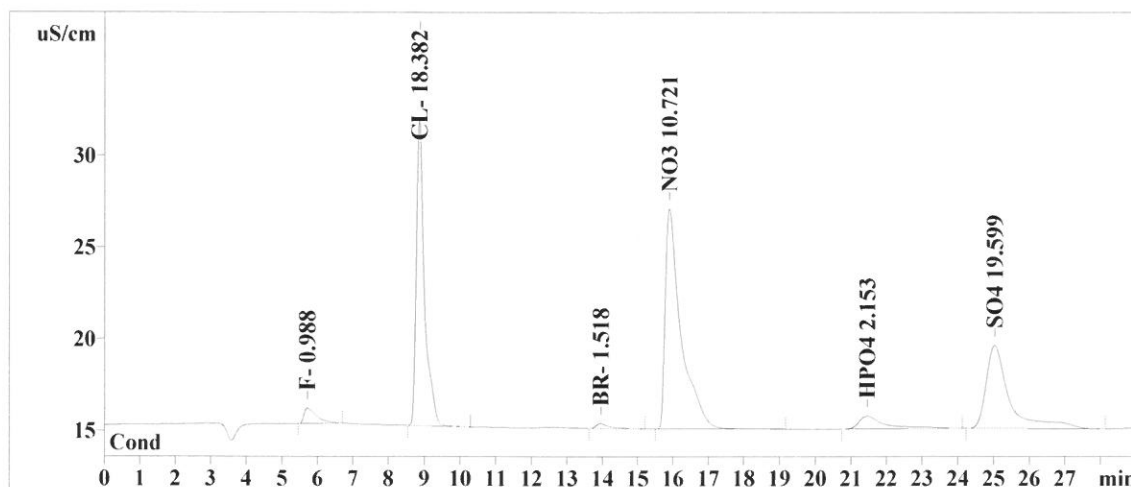

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.351	0.85	2.42	20.690	2.28	0.
2	8.85	0.207	16.76	47.75	262.791	28.97	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	13.95	0.350	0.27	0.77	7.189	0.79	0.
5	15.89	0.408	12.00	34.18	374.792	41.31	0.
6	21.46	0.605	0.70	1.99	36.196	3.99	0.
7	25.02	0.563	4.52	12.89	205.581	22.66	0.
7	29.00	0.355	35.09	99.99	907.239	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:44:32 PM
Printed by: wet


Ident: L4548-01DL2X10
Analysis from: 10/29/2020 3:49:23 PM
File: _2020-10-29_

Last save: 10/29/2020 3:18:12 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72080

Last save: 10/23/2020 12:59:28 PM

SAMPLE: 5.02g/100mL
: AM/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

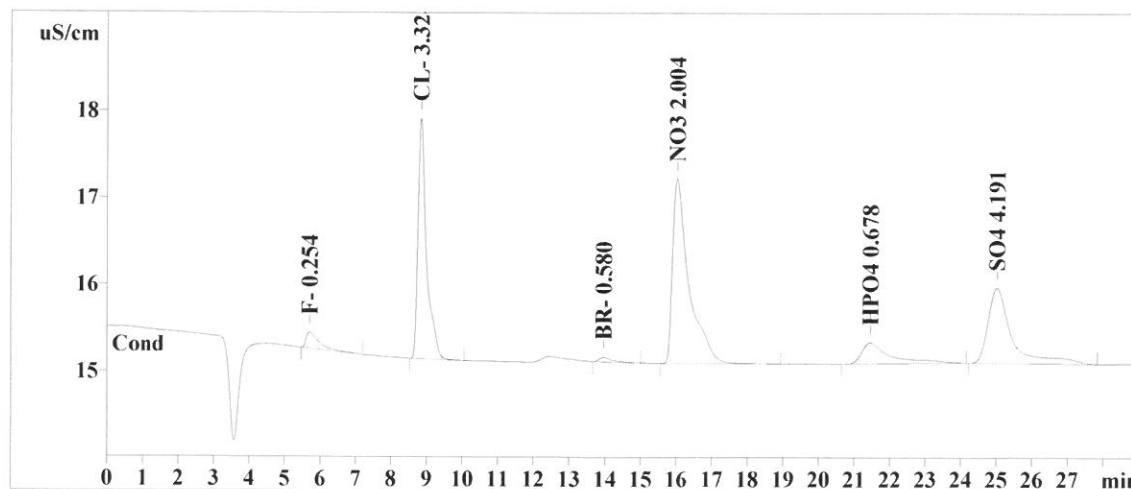

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.70	0.354	0.18	2.96	4.708	2.67	0.
2	8.81	0.224	2.77	44.35	46.641	26.48	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	13.95	0.343	0.05	0.84	1.348	0.76	0.
5	16.01	0.423	2.12	34.03	68.696	38.99	0.
6	21.44	0.674	0.24	3.91	14.130	8.02	0.
7	25.01	0.586	0.86	13.87	40.645	23.07	0.
7	29.00	0.372	6.23	99.96	176.168	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 11/2/2020 1:44:41 PM
 Printed by: wet


Ident: CCV
 Analysis from: 10/29/2020 4:21:35 PM
 File: _2020-10-29_

Last save: 10/29/2020 3:50:24 PM

Method: ANIONS 10-21-20.mtw
 Run operator: wet
 Analysis number: 72081

Last save: 10/23/2020 12:59:28 PM

SAMPLE:
 : AM/AP
 Vial number: 2
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

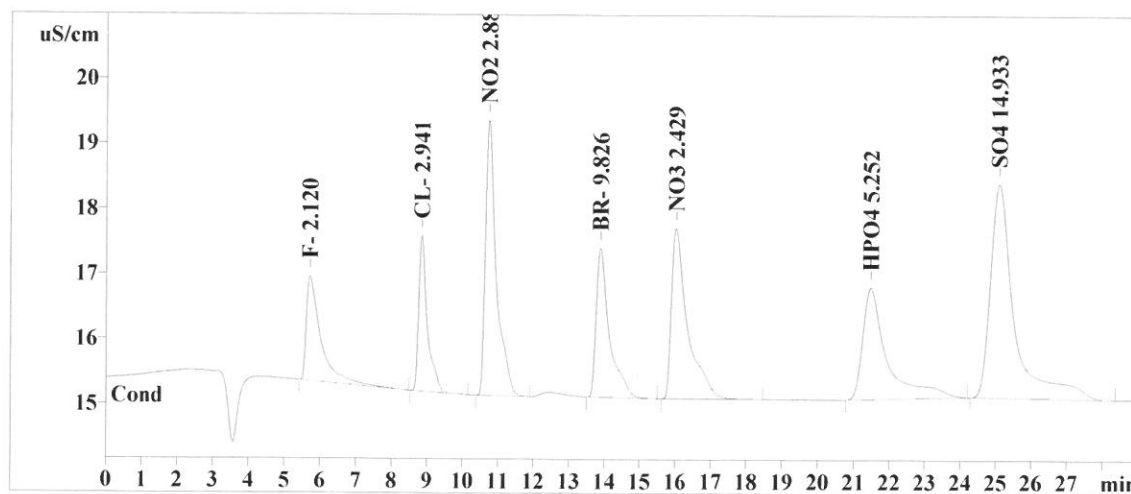

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.366	1.61	8.87	45.343	8.12	0.
2	8.84	0.230	2.38	13.17	41.134	7.36	0.
3	10.72	0.292	4.22	23.32	91.454	16.37	0.
4	13.88	0.335	2.29	12.65	58.920	10.55	0.
5	16.01	0.417	2.61	14.42	83.601	14.97	0.
6	21.47	0.573	1.71	9.45	82.534	14.77	0.
7	25.08	0.593	3.28	18.11	155.636	27.86	0.
7	29.00	0.401	18.10	99.99	558.622	100.00	0.

This report has been created by IC Net
 METROHM LTD

Report date: 11/2/2020 1:44:50 PM
Printed by: wet

Ident: CCB
Analysis from: 10/29/2020 5:05:30 PM
File: _2020-10-29_


Last save: 10/29/2020 4:34:18 PM

Method: ANIONS 10-21-20.mtw
Run operator: wet
Analysis number: 72082

Last save: 10/23/2020 12:59:28 PM

SAMPLE:

: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

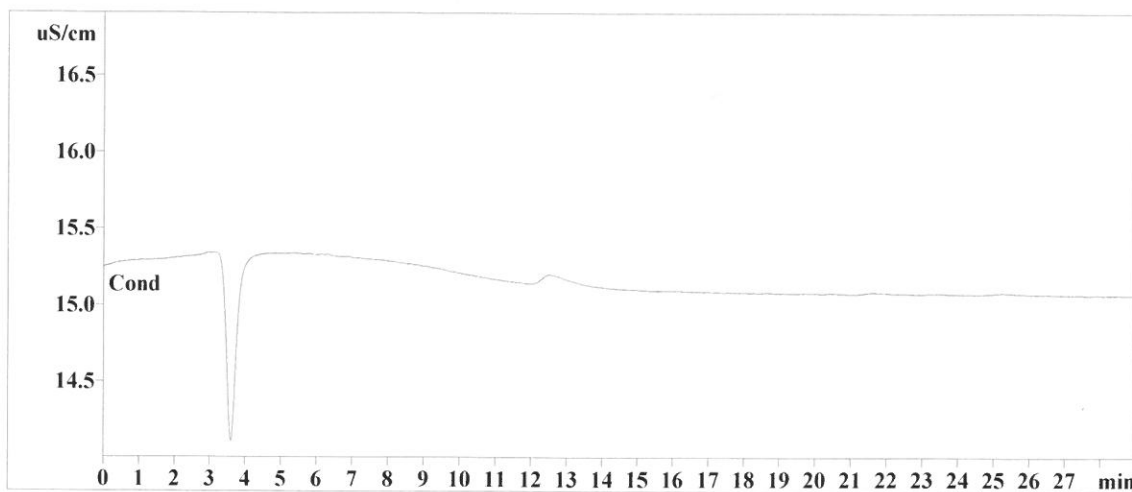

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD