

LB111792

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

11/2/2020 14:45

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.953	0.0	0.085	
ICB1	0.062	0.0	0.000	
CCV1	244.525	0.0	0.217	
CCB1	0.431	0.0	0.001	
PB132776BL	0.425	0.0	0.001	
L4568-01	0.322	0.0	0.001	
L4568-02	0.312	0.0	0.001	
L4222-11	0.028	0.0	0.000	
L4222-11DUP	0.059	0.0	0.000	
CCV2	254.645	0.0	0.226	
CCB2	0.591	0.0	0.001	

N	11
Mean	54.305
SD	100.7002
CV%	185.44

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

11/2/2020 12:36


Test Total CN

Accepted 11/2/2020 12:36

Factor 1127
Bias 0

Coeff. of det. 0.999955

Errors

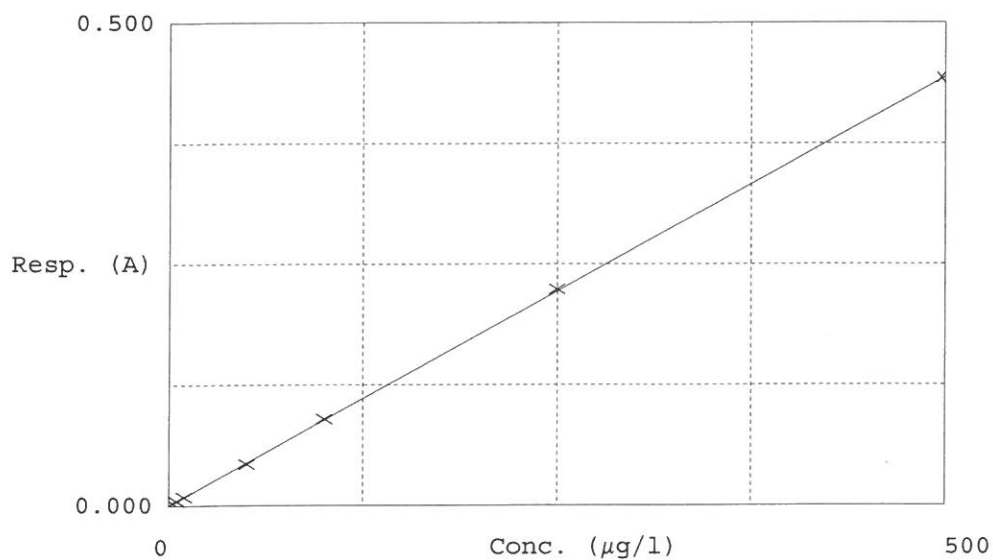

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.0765	0.0000	
2	5.0PPBCN	0.005	5.0099	5.0000	
3	10PPBCN	0.009	9.8435	10.0000	
4	50PPBCN	0.043	48.2092	50.0000	
5	100PPBCN	0.090	100.7872	100.0000	
6	250PPBCN	0.224	252.0979	250.0000	
7	500PPBCN	0.443	498.9757	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 02 14:09:32 2020

Mon Nov 02 14:41:42 2020

Sample Id	Sam/Ctr/c	Test short	nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	CN	P	0.0765	µg/l	11/2/2020 12:28:22	
5.OPPBCN	A	Reactive	CN	P	5.0099	µg/l	11/2/2020 12:28:23	
10PPBCN	A	Reactive	CN	P	9.8435	µg/l	11/2/2020 12:28:24	
50PPBCN	A	Reactive	CN	P	48.2092	µg/l	11/2/2020 12:28:25	
100PPBCN	A	Reactive	CN	P	100.7872	µg/l	11/2/2020 12:28:26	
250PPBCN	A	Reactive	CN	P	252.0979	µg/l	11/2/2020 12:28:27	
500PPBCN	A	Reactive	CN	P	498.9757	µg/l	11/2/2020 12:28:28	
ICV1	S	Reactive	CN	P	95.9526	µg/l	11/2/2020 14:09:33	
ICB1	S	Reactive	CN	P	0.0624	µg/l	11/2/2020 14:09:34	
CCV1	S	Reactive	CN	P	244.5249	µg/l	11/2/2020 14:09:37	
CCB1	S	Reactive	CN	P	0.4309	µg/l	11/2/2020 14:09:38	
PB132776BL	S	Reactive	CN	P	0.4246	µg/l	11/2/2020 14:09:40	
L4568-01	S	Reactive	CN	P	0.3218	µg/l	11/2/2020 14:14:47	
L4568-02	S	Reactive	CN	P	0.3121	µg/l	11/2/2020 14:14:48	
L4222-11	S	Reactive	CN	P	0.0283	µg/l	11/2/2020 14:41:37	
L4222-11DUP	S	Reactive	CN	P	0.0588	µg/l	11/2/2020 14:41:38	
CCV2	S	Reactive	CN	P	254.6453	µg/l	11/2/2020 14:41:40	
CCB2	S	Reactive	CN	P	0.5911	µg/l	11/2/2020 14:41:41	