

LB111837

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

11/4/2020 16:40

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.980	0.0	0.108	
ICB1	0.006	0.0	0.005	
CCV1	0.983	0.0	0.109	
CCB1	0.006	0.0	0.005	
PB132826BL	0.008	0.0	0.005	
PB132826BS	0.990	0.0	0.109	
L4612-01	0.003	0.0	0.005	
L4612-01DUP	0.004	0.0	0.005	
L4612-01MS	0.891	0.0	0.099	
L4612-01MSD	0.884	0.0	0.098	
CCV2	0.993	0.0	0.110	
CCB2	0.008	0.0	0.005	

N	12
Mean	0.480
SD	0.4961
CV%	103.41

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 04 16:04:54 2020

Wed Nov 04 16:39:49 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0512	mg/l	11/4/2020 16:04:54	
0.1PPM	A	Phenolics-	P	0.0964	mg/l	11/4/2020 16:04:55	
0.25PPM	A	Phenolics-	P	0.2508	mg/l	11/4/2020 16:04:56	
0.50PPM	A	Phenolics-	P	0.5022	mg/l	11/4/2020 16:04:57	
1.0PPM	A	Phenolics-	P	0.9998	mg/l	11/4/2020 16:04:58	
2.0PPM	A	Phenolics-	P	1.9996	mg/l	11/4/2020 16:04:59	
ICV1	S	Phenolics-	P	0.9802	mg/l	11/4/2020 16:32:28	
ICB1	S	Phenolics-	P	0.0063	mg/l	11/4/2020 16:32:29	
CCV1	S	Phenolics-	P	0.983	mg/l	11/4/2020 16:32:32	
CCB1	S	Phenolics-	P	0.0057	mg/l	11/4/2020 16:32:33	
PB132826BL	S	Phenolics-	P	0.0078	mg/l	11/4/2020 16:32:35	
PB132826BS	S	Phenolics-	P	0.9896	mg/l	11/4/2020 16:32:36	
L4612-01	S	Phenolics-	P	0.0033	mg/l	11/4/2020 16:32:37	
L4612-01DUP	S	Phenolics-	P	0.0043	mg/l	11/4/2020 16:32:38	
L4612-01MS	S	Phenolics-	P	0.8913	mg/l	11/4/2020 16:39:41	
L4612-01MSD	S	Phenolics-	P	0.884	mg/l	11/4/2020 16:39:42	
CCV2	S	Phenolics-	P	0.9933	mg/l	11/4/2020 16:39:46	
CCB2	S	Phenolics-	P	0.0082	mg/l	11/4/2020 16:39:47	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

11/4/2020 16:05


Test Phenolics-

Accepted 11/4/2020 16:05

Factor 9.42
Bias 0.004

Coeff. of det. 0.999993

Errors

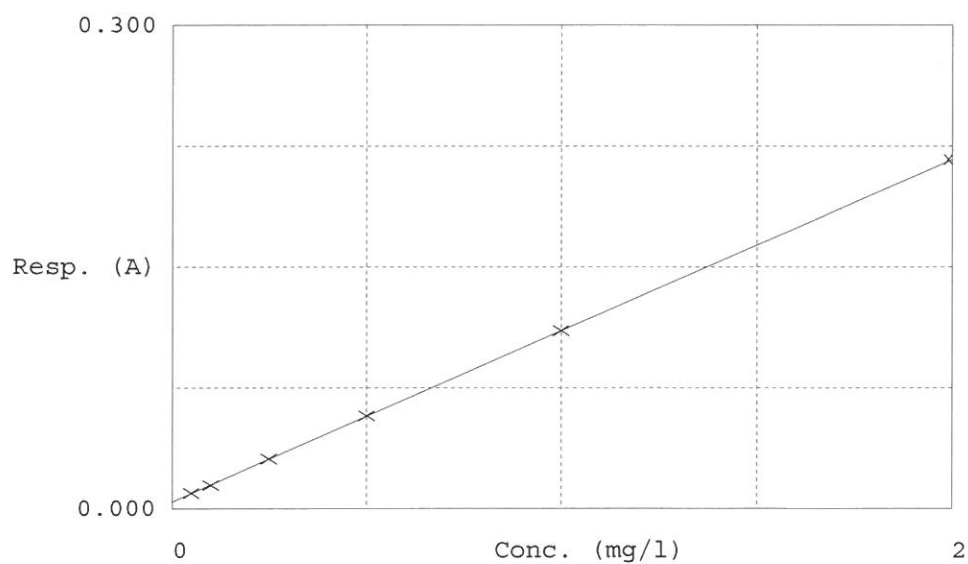

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.010	0.0512	0.0500	
2	Phenol-2	0.015	0.0964	0.1000	
3	Phenol-2	0.031	0.2508	0.2500	
4	Phenol-2	0.058	0.5022	0.5000	
5	Phenol-2	0.110	0.9998	1.0000	
6	Phenol-2	0.217	1.9996	2.0000	