

LB111850

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Am

Instrument ID : Konelab

11/5/2020 14:14

Test: Ammonia-N

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.962	0.0	0.226	
ICB1	0.020	0.0	0.026	
CCV1	0.934	0.0	0.220	
CCB1	0.023	0.0	0.026	
PB132839BL	0.020	0.0	0.026	
PB132839BS	0.926	0.0	0.218	
L4612-01	0.138	0.0	0.051	
L4612-01DUP	0.132	0.0	0.049	
L4612-01MS	0.793	0.0	0.190	
L4612-01MSD	0.813	0.0	0.194	
CCV2	0.965	0.0	0.226	
CCB2	0.023	0.0	0.026	

N	12
Mean	0.479
SD	0.4432
CV%	92.50

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

11/5/2020 12:50


Test Ammonia-N

Accepted 11/5/2020 12:50

Factor 4.704
Bias 0.021

Coeff. of det. 0.999718

Errors

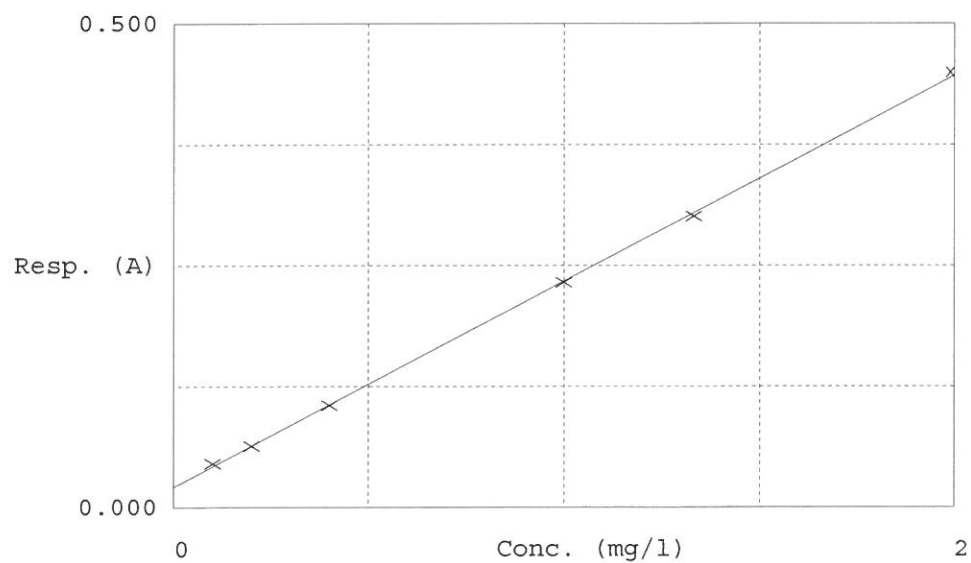

	Calibrator	Response	Calc. con.	Conc.	Errors
1	NH3-2PPM	0.045	0.1135	0.1000	
2	NH3-2PPM	0.064	0.1987	0.2000	
3	NH3-2PPM	0.106	0.3970	0.4000	
4	NH3-2PPM	0.232	0.9932	1.0000	
5	NH3-2PPM	0.301	1.3158	1.3333	
6	NH3-2PPM	0.450	2.0152	2.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Nov 05 12:49:37 2020

Thu Nov 05 14:01:26 2020

Sample Id	Sam/Ctr/c/	Test short Test type	Result	Result unit	Result date and time	Stat
0.1PPM	A	Ammonia-I P	0.1135	mg/l	11/5/2020 12:49:37	
0.2PPM	A	Ammonia-I P	0.1987	mg/l	11/5/2020 12:49:38	
0.4PPM	A	Ammonia-I P	0.397	mg/l	11/5/2020 12:49:39	
1.0PPM	A	Ammonia-I P	0.9932	mg/l	11/5/2020 12:49:40	
1.3PPM	A	Ammonia-I P	1.3158	mg/l	11/5/2020 12:49:41	
2.0PPM	A	Ammonia-I P	2.0152	mg/l	11/5/2020 12:49:42	
ICV1	S	Ammonia-I P	0.9623	mg/l	11/5/2020 13:25:28	
ICB1	S	Ammonia-I P	0.0202	mg/l	11/5/2020 13:25:29	
CCV1	S	Ammonia-I P	0.9344	mg/l	11/5/2020 13:25:32	
CCB1	S	Ammonia-I P	0.0227	mg/l	11/5/2020 13:25:33	
PB132839BL	S	Ammonia-I P	0.0203	mg/l	11/5/2020 13:25:35	
PB132839BS	S	Ammonia-I P	0.9256	mg/l	11/5/2020 13:25:36	
L4612-01	S	Ammonia-I P	0.138	mg/l	11/5/2020 13:25:37	
L4612-01DUP	S	Ammonia-I P	0.1323	mg/l	11/5/2020 13:25:38	
L4612-01MS	S	Ammonia-I P	0.7928	mg/l	11/5/2020 13:34:28	
L4612-01MSD	S	Ammonia-I P	0.8133	mg/l	11/5/2020 13:34:29	
CCV2	S	Ammonia-I P	0.9651	mg/l	11/5/2020 13:34:30	
CCB2	S	Ammonia-I P	0.0226	mg/l	11/5/2020 13:34:32	