

LB112029

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

11/18/2020 14:33

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.114	0.0	0.089	
ICB1	-0.726	0.0	0.000	
CCV1	248.223	0.0	0.225	
CCB1	-0.391	0.0	0.001	
PB133087BL	-0.499	0.0	0.001	
L4765-01	-0.756	0.0	0.000	
L4765-01DUP	-0.649	0.0	0.001	
L4765-03	-0.728	0.0	0.000	
L4776-02	-0.734	0.0	0.000	
L4777-01	-1.436	0.0	-0.000	
PB133088BL	-0.850	0.0	0.000	
L4775-01	-0.834	0.0	0.000	
L4775-01DUP	-0.264	0.0	0.001	
CCV2	249.649	0.0	0.226	
CCB2	-0.316	0.0	0.001	

N	15
Mean	39.120
SD	88.8100
CV%	227.02

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 18 14:23:10 2020

Wed Nov 18 14:30:26 2020

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	0.004	µg/l	11/18/2020 11:59:32
5.OPPBCN	A	Reactive CN	P	4.1626	µg/l	11/18/2020 11:59:33
10PPBCN	A	Reactive CN	P	9.1942	µg/l	11/18/2020 11:59:34
50PPBCN	A	Reactive CN	P	49.5773	µg/l	11/18/2020 11:59:35
100PPBCN	A	Reactive CN	P	100.4796	µg/l	11/18/2020 11:59:36
250PPBCN	A	Reactive CN	P	253.2231	µg/l	11/18/2020 11:59:37
500PPBCN	A	Reactive CN	P	498.3593	µg/l	11/18/2020 11:59:38
ICV1	S	Reactive CN	P	97.1136	µg/l	11/18/2020 14:23:11
ICB1	S	Reactive CN	P	-0.7255	µg/l	11/18/2020 14:23:12
CCV1	S	Reactive CN	P	248.2228	µg/l	11/18/2020 14:23:15
CCB1	S	Reactive CN	P	-0.3912	µg/l	11/18/2020 14:23:16
PB133087BL	S	Reactive CN	P	-0.4993	µg/l	11/18/2020 14:23:18
L4765-01	S	Reactive CN	P	-0.7561	µg/l	11/18/2020 14:23:19
L4765-01DUP	S	Reactive CN	P	-0.6487	µg/l	11/18/2020 14:23:20
L4765-03	S	Reactive CN	P	-0.7278	µg/l	11/18/2020 14:30:17
L4776-02	S	Reactive CN	P	-0.7338	µg/l	11/18/2020 14:30:18
L4777-01	S	Reactive CN	P	-1.4364	µg/l	11/18/2020 14:30:19
PB133088BL	S	Reactive CN	P	-0.8503	µg/l	11/18/2020 14:30:20
L4775-01	S	Reactive CN	P	-0.8341	µg/l	11/18/2020 14:30:21
L4775-01DUP	S	Reactive CN	P	-0.2638	µg/l	11/18/2020 14:30:22
CCV2	S	Reactive CN	P	249.6488	µg/l	11/18/2020 14:30:24
CCB2	S	Reactive CN	P	-0.3157	µg/l	11/18/2020 14:30:25

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Am

Instrument ID : Konelab

11/18/2020 12:05


Test Total CN

Accepted 11/18/2020 12:05

Factor 1108
Bias 0.001

Coeff. of det. 0.999928

Errors

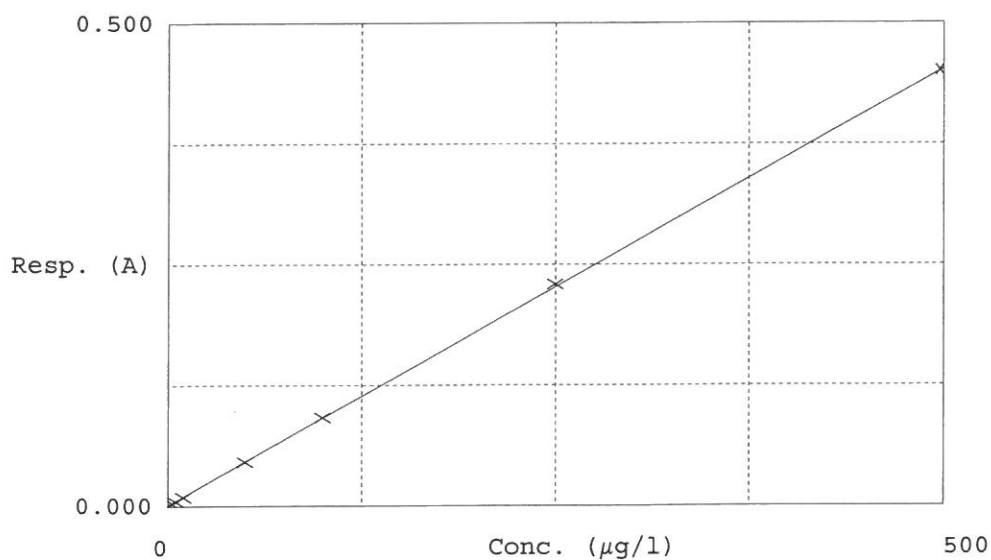

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.0040	0.0000	
2	5.0PPBCN	0.005	4.1626	5.0000	
3	10PPBCN	0.009	9.1942	10.0000	
4	50PPBCN	0.046	49.5773	50.0000	
5	100PPBCN	0.092	100.4796	100.0000	
6	250PPBCN	0.230	253.2231	250.0000	
7	500PPBCN	0.451	498.3593	500.0000	