

LB112171

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

11/30/2020 15:20

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.459	0.0	0.081	
ICB1	0.952	0.0	0.001	
CCV1	244.588	0.0	0.212	
CCB1	0.867	0.0	0.001	
PB133306BL	0.691	0.0	0.000	
L4900-04	0.369	0.0	0.000	
L4900-06	0.753	0.0	0.000	
L4903-04	0.578	0.0	0.000	
L4903-08	0.836	0.0	0.001	
L4899-04	0.580	0.0	0.000	
L4899-04DUP	0.706	0.0	0.000	
CCV2	258.499	0.0	0.224	
CCB2	0.845	0.0	0.001	

N	13
Mean	46.440
SD	94.5815
CV%	203.66

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 30 14:23:56 2020

Mon Nov 30 15:20:13 2020

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.0PPBCN	A	Reactive CN	P	0.4856	µg/l	11/30/2020 14:23:56
5.0PPBCN	A	Reactive CN	P	4.9238	µg/l	11/30/2020 14:23:57
10PPBCN	A	Reactive CN	P	10.8801	µg/l	11/30/2020 14:23:58
50PPBCN	A	Reactive CN	P	48.3324	µg/l	11/30/2020 14:23:59
100PPBCN	A	Reactive CN	P	97.9972	µg/l	11/30/2020 14:24:00
250PPBCN	A	Reactive CN	P	253.6611	µg/l	11/30/2020 14:24:01
500PPBCN	A	Reactive CN	P	498.7199	µg/l	11/30/2020 14:24:02
ICV1	S	Reactive CN	P	93.459	µg/l	11/30/2020 14:53:43
ICB1	S	Reactive CN	P	0.9519	µg/l	11/30/2020 14:53:44
CCV1	S	Reactive CN	P	244.5877	µg/l	11/30/2020 14:53:47
CCB1	S	Reactive CN	P	0.8669	µg/l	11/30/2020 14:53:48
PB133306BL	S	Reactive CN	P	0.6909	µg/l	11/30/2020 14:53:50
L4900-04	S	Reactive CN	P	0.3689	µg/l	11/30/2020 14:59:52
L4900-06	S	Reactive CN	P	0.7526	µg/l	11/30/2020 14:59:53
L4903-04	S	Reactive CN	P	0.5784	µg/l	11/30/2020 14:59:54
L4903-08	S	Reactive CN	P	0.8363	µg/l	11/30/2020 14:59:55
L4899-04	S	Reactive CN	P	0.58	µg/l	11/30/2020 15:20:10
L4899-04DUP	S	Reactive CN	P	0.7057	µg/l	11/30/2020 15:20:11
CCV2	S	Reactive CN	P	258.4989	µg/l	11/30/2020 15:20:12
CCB2	S	Reactive CN	P	0.8449	µg/l	11/30/2020 15:20:13

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

11/30/2020 14:28


Test Total CN

Accepted 11/30/2020 14:24

Factor 1151
Bias 0

Coeff. of det. 0.999889

Errors

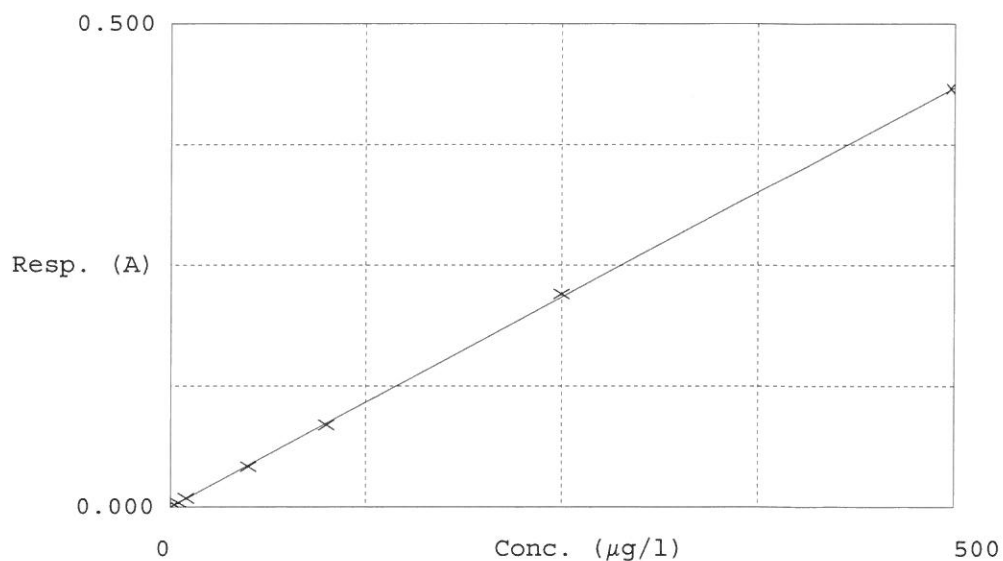

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.4856	0.0000	
2	5.0PPBCN	0.004	4.9238	5.0000	
3	10PPBCN	0.009	10.8801	10.0000	
4	50PPBCN	0.042	48.3324	50.0000	
5	100PPBCN	0.085	97.9972	100.0000	
6	250PPBCN	0.220	253.6611	250.0000	
7	500PPBCN	0.433	498.7199	500.0000	