

LB112284

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

12/9/2020 13:33

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.616	0.0	0.089	
ICB1	0.489	0.0	0.001	
CCV1	241.138	0.0	0.224	
CCB1	0.321	0.0	0.001	
PB133465BL	0.471	0.0	0.001	
L4965-02	0.213	0.0	0.000	
L4965-07	0.269	0.0	0.000	
L4965-12	0.255	0.0	0.000	
L4966-02	0.547	0.0	0.001	
L4913-02	0.150	0.0	0.000	
L4913-02DUP	0.094	0.0	0.000	
CCV2	251.140	0.0	0.234	
CCB2	0.682	0.0	0.001	

N	13
Mean	45.491
SD	92.8529
CV%	204.11

Aquakem v. 7.2AQ1

Results from time period:

Wed Dec 09 12:49:44 2020

Wed Dec 09 13:23:41 2020

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.1686	µg/l	12/9/2020 10:25:39	
5.OPPBCN	A	Reactive CN	P	4.8992	µg/l	12/9/2020 10:25:40	
10PPBCN	A	Reactive CN	P	10.1143	µg/l	12/9/2020 10:25:41	
50PPBCN	A	Reactive CN	P	49.8974	µg/l	12/9/2020 10:25:42	
100PPBCN	A	Reactive CN	P	99.4565	µg/l	12/9/2020 10:25:43	
250PPBCN	A	Reactive CN	P	250.6926	µg/l	12/9/2020 10:25:44	
500PPBCN	A	Reactive CN	P	499.7714	µg/l	12/9/2020 10:25:45	
ICV1	S	Reactive CN	P	95.6164	µg/l	12/9/2020 12:49:45	
ICB1	S	Reactive CN	P	0.4886	µg/l	12/9/2020 12:49:46	
CCV1	S	Reactive CN	P	241.138	µg/l	12/9/2020 12:49:49	
CCB1	S	Reactive CN	P	0.3215	µg/l	12/9/2020 12:49:50	
PB133465BL	S	Reactive CN	P	0.4711	µg/l	12/9/2020 12:49:52	
L4965-02	S	Reactive CN	P	0.2126	µg/l	12/9/2020 12:55:56	
L4965-07	S	Reactive CN	P	0.2686	µg/l	12/9/2020 12:55:57	
L4965-12	S	Reactive CN	P	0.2552	µg/l	12/9/2020 12:55:58	
L4966-02	S	Reactive CN	P	0.5472	µg/l	12/9/2020 12:55:59	
L4913-02	S	Reactive CN	P	0.1504	µg/l	12/9/2020 13:23:35	
L4913-02DUP	S	Reactive CN	P	0.0942	µg/l	12/9/2020 13:23:36	
CCV2	S	Reactive CN	P	251.1398	µg/l	12/9/2020 13:23:39	
CCB2	S	Reactive CN	P	0.6817	µg/l	12/9/2020 13:23:40	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : PM

Instrument ID : Konelab

12/9/2020 10:37


Test Total CN

Accepted 12/9/2020 10:37

Factor 1075
Bias 0

Coeff. of det. 0.999996

Errors

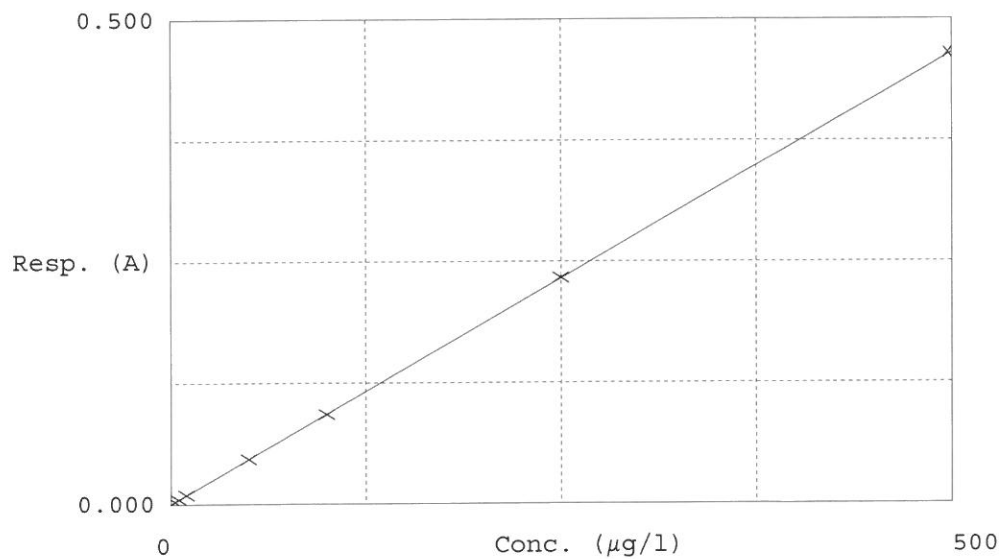

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.1686	0.0000	
2	5.0PPBCN	0.005	4.8992	5.0000	
3	10PPBCN	0.010	10.1143	10.0000	
4	50PPBCN	0.047	49.8974	50.0000	
5	100PPBCN	0.093	99.4565	100.0000	
6	250PPBCN	0.233	250.6926	250.0000	
7	500PPBCN	0.465	499.7714	500.0000	