

LB112488

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

12/22/2020 11:50

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.883	0.0	0.088	
ICB1	0.457	0.0	0.000	
CCV1	240.638	0.0	0.226	
CCB1	0.502	0.0	0.000	
PB133727BL	0.696	0.0	0.001	
PB133727BS	96.375	0.0	0.091	
LOWPB133727	9.975	0.0	0.009	
HIGHPB133727	470.955	0.0	0.443	
L5126-02	8.201	0.0	0.008	
L5126-02DUP	8.199	0.0	0.008	
L5126-02MS	41.580	0.0	0.039	
L5126-02MSD	41.779	0.0	0.039	
CCV2	243.092	0.0	0.228	
CCB2	0.822	0.0	0.001	

N	14
Mean	89.797
SD	138.0420
CV%	153.73

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

12/22/2020 11:04


Test Total CN

Accepted 12/22/2020 11:04

Factor 1064
Bias 0

Coeff. of det. 0.999991

Errors

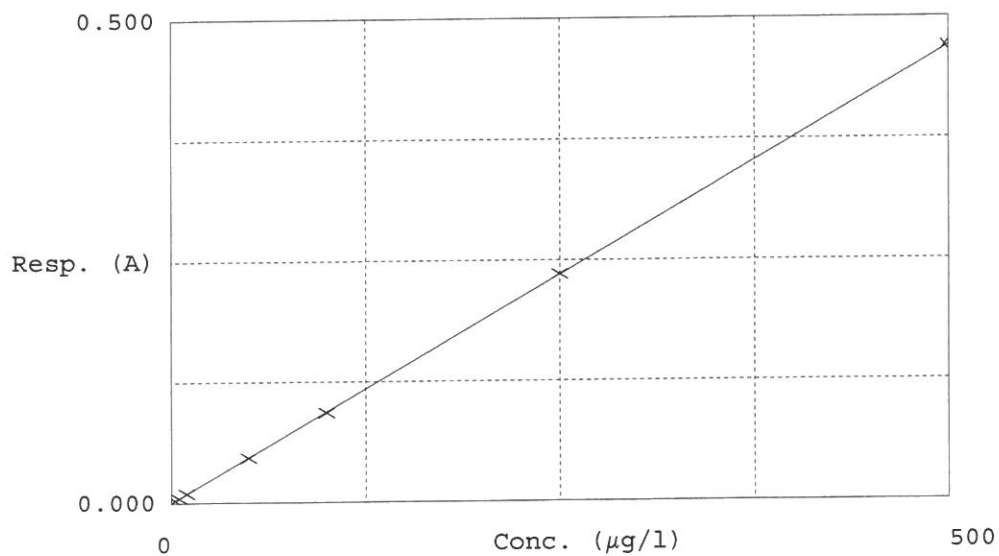

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.3156	0.0000	
2	5.0PPBCN	0.005	5.2460	5.0000	
3	10PPBCN	0.010	10.5186	10.0000	
4	50PPBCN	0.046	49.3570	50.0000	
5	100PPBCN	0.093	99.1137	100.0000	
6	250PPBCN	0.235	250.4408	250.0000	
7	500PPBCN	0.470	500.0083	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Tue Dec 22 10:41:39 2020

Tue Dec 22 11:42:41 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.3156	µg/l	12/22/2020 11:03:49	
5.OPPBCN	A	Total CN	P	5.246	µg/l	12/22/2020 11:03:50	
10PPBCN	A	Total CN	P	10.5186	µg/l	12/22/2020 11:03:51	
50PPBCN	A	Total CN	P	49.357	µg/l	12/22/2020 11:03:52	
100PPBCN	A	Total CN	P	99.1137	µg/l	12/22/2020 11:03:53	
250PPBCN	A	Total CN	P	250.4408	µg/l	12/22/2020 11:03:54	
500PPBCN	A	Total CN	P	500.0083	µg/l	12/22/2020 11:03:55	
ICV1	S	Total CN	P	93.8826	µg/l	12/22/2020 11:32:19	
ICB1	S	Total CN	P	0.4567	µg/l	12/22/2020 11:32:20	
CCV1	S	Total CN	P	240.6382	µg/l	12/22/2020 11:32:23	
CCB1	S	Total CN	P	0.5024	µg/l	12/22/2020 11:32:24	
PB133727BL	S	Total CN	P	0.6964	µg/l	12/22/2020 11:32:26	
PB133727BS	S	Total CN	P	96.3753	µg/l	12/22/2020 11:32:27	
LOWPB133727	S	Total CN	P	9.9751	µg/l	12/22/2020 11:32:28	
HIGHPB133727	S	Total CN	P	470.9546	µg/l	12/22/2020 11:39:53	
L5126-02	S	Total CN	P	8.2006	µg/l	12/22/2020 11:39:54	
L5126-02DUP	S	Total CN	P	8.1987	µg/l	12/22/2020 11:39:55	
L5126-02MS	S	Total CN	P	41.58	µg/l	12/22/2020 11:39:56	
L5126-02MSD	S	Total CN	P	41.7794	µg/l	12/22/2020 11:39:57	
CCV2	S	Total CN	P	243.0924	µg/l	12/22/2020 11:40:01	
CCB2	S	Total CN	P	0.822	µg/l	12/22/2020 11:40:02	