

LB112492

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

12/22/2020 13:21

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.491	0.0	0.089	
ICB1	0.567	0.0	0.000	
CCV1	243.356	0.0	0.229	
CCB1	0.589	0.0	0.000	
PB133669BL	0.329	0.0	0.000	
PB133669BS	95.970	0.0	0.090	
MIDPB133669	241.403	0.0	0.227	
L4981-02	1.614	0.0	0.001	
L4981-02DUP	1.775	0.0	0.002	
L4981-02MS	29.545	0.0	0.028	
L4981-02MSD	29.245	0.0	0.027	
L5153-07	7.372	0.0	0.007	
L5174-07	6.507	0.0	0.006	
L4981-02A	37.125	0.0	0.035	
CCV3	244.038	0.0	0.229	
CCB3	0.604	0.0	0.000	

N	16
Mean	64.658
SD	93.6340
CV%	144.81

Aquakem v. 7.2AQ1

Results from time period:

Tue Dec 22 12:55:50 2020

Tue Dec 22 13:09:43 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.3156	µg/l	12/22/2020 11:03:49	
5.OPPBCN	A	Total CN	P	5.246	µg/l	12/22/2020 11:03:50	
10PPBCN	A	Total CN	P	10.5186	µg/l	12/22/2020 11:03:51	
50PPBCN	A	Total CN	P	49.357	µg/l	12/22/2020 11:03:52	
100PPBCN	A	Total CN	P	99.1137	µg/l	12/22/2020 11:03:53	
250PPBCN	A	Total CN	P	250.4408	µg/l	12/22/2020 11:03:54	
500PPBCN	A	Total CN	P	500.0083	µg/l	12/22/2020 11:03:55	
ICV1	S	Total CN	P	94.4905	µg/l	12/22/2020 12:55:51	
ICB1	S	Total CN	P	0.5669	µg/l	12/22/2020 12:55:52	
CCV1	S	Total CN	P	243.3557	µg/l	12/22/2020 12:55:55	
CCB1	S	Total CN	P	0.5893	µg/l	12/22/2020 12:55:56	
PB133669BL	S	Total CN	P	0.3295	µg/l	12/22/2020 12:55:58	
PB133669BS	S	Total CN	P	95.9695	µg/l	12/22/2020 12:55:59	
MIDPB133669	S	Total CN	P	241.4025	µg/l	12/22/2020 12:56:00	
L4981-02	S	Total CN	P	1.6142	µg/l	12/22/2020 13:03:25	
L4981-02DUP	S	Total CN	P	1.7748	µg/l	12/22/2020 13:03:26	
L4981-02MS	S	Total CN	P	29.545	µg/l	12/22/2020 13:03:29	
L4981-02MSD	S	Total CN	P	29.2447	µg/l	12/22/2020 13:03:30	
L5153-07	S	Total CN	P	7.3724	µg/l	12/22/2020 13:03:31	
L5174-07	S	Total CN	P	6.5071	µg/l	12/22/2020 13:03:32	
L4981-02A	S	Total CN	P	37.1251	µg/l	12/22/2020 13:09:38	
CCV3	S	Total CN	P	244.0383	µg/l	12/22/2020 13:09:41	
CCB3	S	Total CN	P	0.6036	µg/l	12/22/2020 13:09:42	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AM

Instrument ID : Konelab

12/22/2020 11:04


Test Total CN

Accepted 12/22/2020 11:04

Factor 1064
 Bias 0

Coeff. of det. 0.999991

Errors

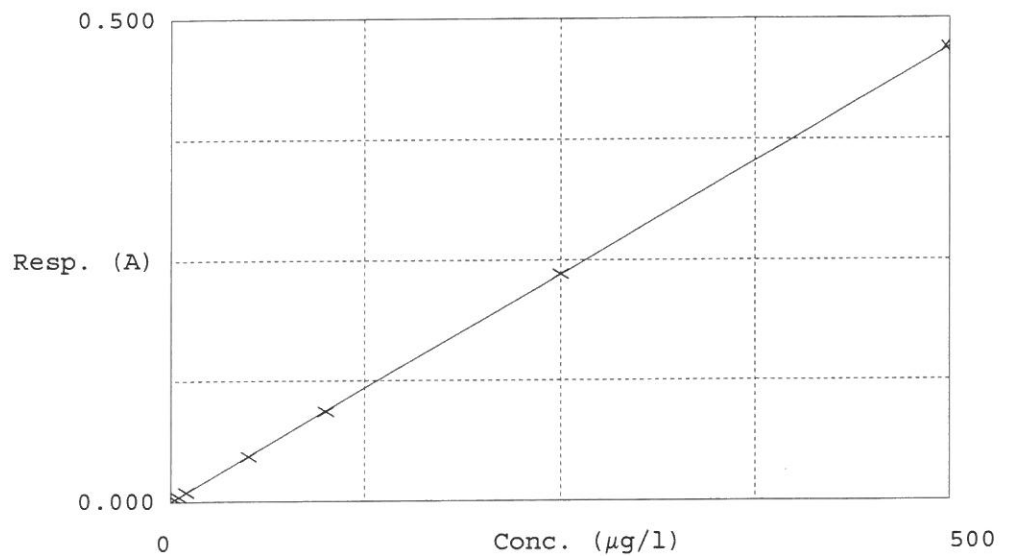

	Calibrator	Response	Calc. con.	Conc.	Errors	%
1	0.0PPBCN	0.000	0.3156	0.0000		105
2	5.0PPBCN	0.005	5.2460	5.0000		105
3	10PPBCN	0.010	10.5186	10.0000		98
4	50PPBCN	0.046	49.3570	50.0000		99
5	100PPBCN	0.093	99.1137	100.0000		100
6	250PPBCN	0.235	250.4408	250.0000		100
7	500PPBCN	0.470	500.0083	500.0000		100

12/22/2020
 AM