

LB113102

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

3/8/2021 16:54

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.982	0.0	0.111	
ICB1	-0.003	0.0	0.006	
CCV1	0.986	0.0	0.112	
CCB1	-0.001	0.0	0.006	
PB134989BL	0.003	0.0	0.006	
PB134989BS	0.985	0.0	0.112	
M1458-01	0.022	0.0	0.008	
M1458-02	0.044	0.0	0.011	
PB134991BL	-0.001	0.0	0.006	
PB134991BS	0.980	0.0	0.111	
M1458-07	0.023	0.0	0.008	
M1458-08	0.042	0.0	0.010	
M1561-26	2.368	0.0	0.261	Test limit high
M1561-26DLX2	1.195	0.0	0.134	
CCV2	0.985	0.0	0.112	
CCB2	-0.001	0.0	0.006	

N	16
Mean	0.538
SD	0.6949
CV%	129.17

Aquakem v. 7.2AQ1

Results from time period:

Mon Mar 08 16:33:47 2021

Mon Mar 08 16:51:40 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPM	A	Phenolics-	P	0.0011	mg/l	3/8/2021 14:31:58	
0.05PPM	A	Phenolics-	P	0.0574	mg/l	3/8/2021 14:31:59	
0.1PPM	A	Phenolics-	P	0.1035	mg/l	3/8/2021 14:32:00	
0.25PPM	A	Phenolics-	P	0.2452	mg/l	3/8/2021 14:32:01	
0.50PPM	A	Phenolics-	P	0.5054	mg/l	3/8/2021 14:32:02	
1.OPPM	A	Phenolics-	P	0.9768	mg/l	3/8/2021 14:32:03	
2.OPPM	A	Phenolics-	P	2.0105	mg/l	3/8/2021 14:32:04	
ICV1	S	Phenolics-	P	0.9816	mg/l	3/8/2021 16:33:48	
ICB1	S	Phenolics-	P	-0.003	mg/l	3/8/2021 16:33:49	
CCV1	S	Phenolics-	P	0.9855	mg/l	3/8/2021 16:33:52	
CCB1	S	Phenolics-	P	-0.0012	mg/l	3/8/2021 16:33:54	
PB134989BL	S	Phenolics-	P	0.0029	mg/l	3/8/2021 16:33:55	
PB134989BS	S	Phenolics-	P	0.985	mg/l	3/8/2021 16:33:57	
M1458-01	S	Phenolics-	P	0.0221	mg/l	3/8/2021 16:43:50	
M1458-02	S	Phenolics-	P	0.0441	mg/l	3/8/2021 16:43:51	
PB134991BL	S	Phenolics-	P	-0.0009	mg/l	3/8/2021 16:43:53	
PB134991BS	S	Phenolics-	P	0.9803	mg/l	3/8/2021 16:43:56	
M1458-07	S	Phenolics-	P	0.0229	mg/l	3/8/2021 16:43:57	
M1458-08	S	Phenolics-	P	0.0421	mg/l	3/8/2021 16:44:00	
M1561-26	S	Phenolics-	P	2.3678	mg/l	3/8/2021 16:51:34	
M1561-26DLX2	S	Phenolics-	P	1.1947	mg/l	3/8/2021 16:51:36	
CCV2	S	Phenolics-	P	0.9849	mg/l	3/8/2021 16:51:38	
CCB2	S	Phenolics-	P	-0.0013	mg/l	3/8/2021 16:51:39	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

3/8/2021 14:33


Test Phenolics-

Accepted 3/8/2021 14:33

Factor 9.297
Bias 0.006

Coeff. of det. 0.999757

Errors

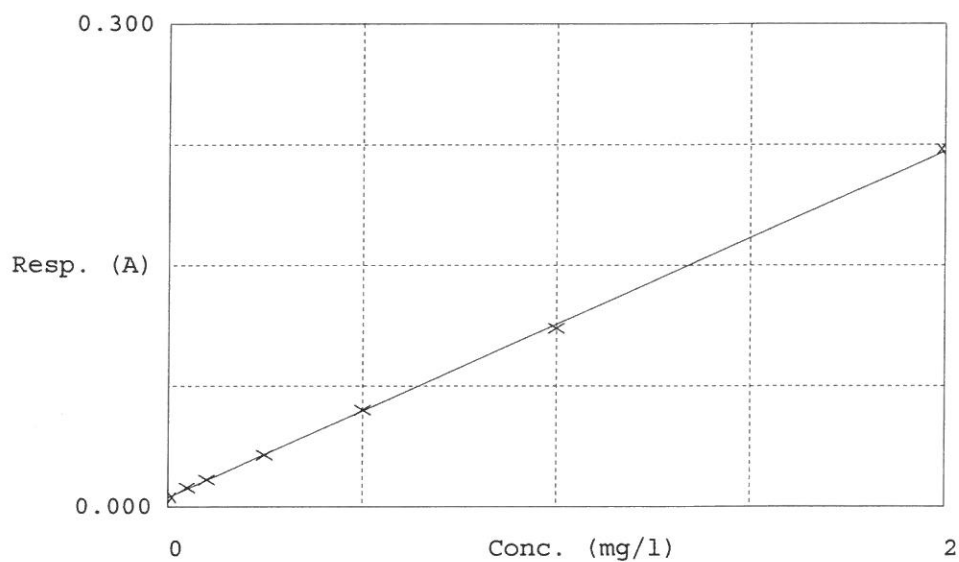

	Calibrator	Response	Calc. con.	Conc.	Errors %D
1	0.00PPM	0.006	0.0011	0.0000	
2	Phenol-2	0.012	0.0574	0.0500	
3	Phenol-2	0.017	0.1035	0.1000	
4	Phenol-2	0.032	0.2452	0.2500	
5	Phenol-2	0.060	0.5054	0.5000	
6	Phenol-2	0.111	0.9768	1.0000	
7	Phenol-2	0.222	2.0105	2.0000	

15
4
2
1
2
1

03/08/2021
AM