


LA114962

7471B

INSTRUMENT ID: CV2

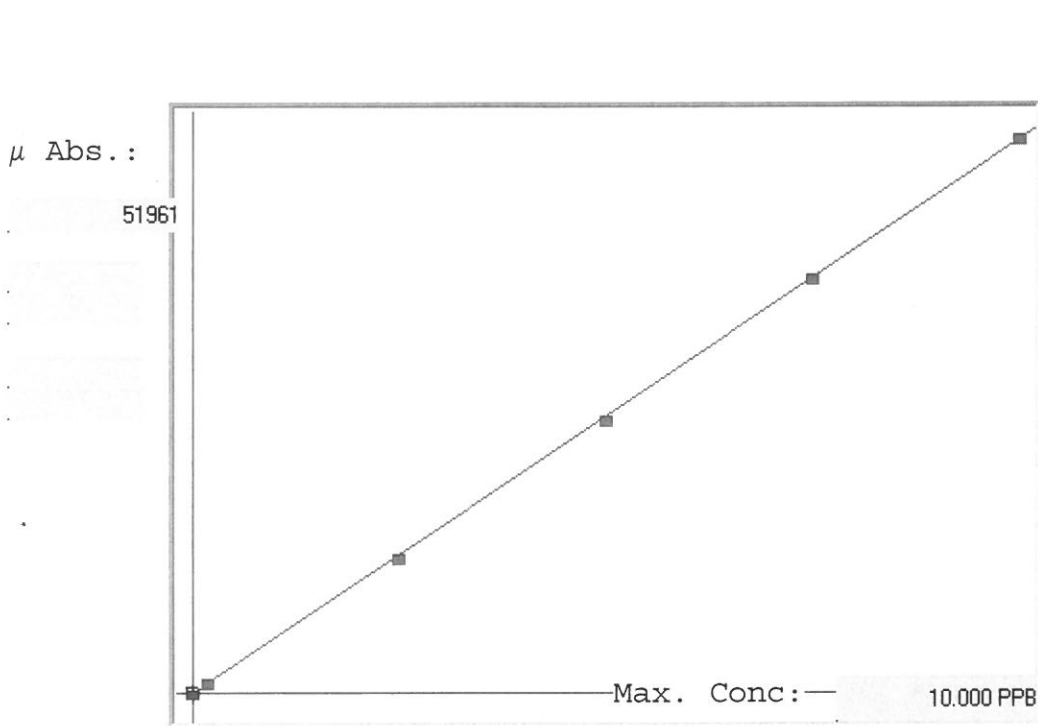

Linear

A= 0.0000e+000

B= 1.9242e-004

C= 2.3652e-002

Rho= 0.9999622

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	921)
0.0	0.000	0.033	0.033	51	0.000	51					181100
0.2	0.200	0.215	0.015	995	0.0 %	995					
2.5	2.500	2.467	-0.033	12699	0.0 %	12699					
5.0	5.000	4.945	-0.055	25579	0.0 %	25579					
7.5	7.500	7.517	0.017	38944	0.0 %	38944					
10.0	10.000	10.022	0.022	51961	0.0 %	51961					

