

LB120437

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : PM Instrument ID : Konelab

6/13/2022 13:27

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.085	0.0	0.073	
ICB1	0.469	0.0	0.001	
CCV1	244.548	0.0	0.189	
CCB1	0.403	0.0	0.001	
PB145491BL	0.341	0.0	0.001	
PB145491BS	94.161	0.0	0.074	
LOWPB145491	9.835	0.0	0.009	489% (10 - 110)
HIGHPB145491	487.794	0.0	0.377	98% (10 - 110)
N3304-01	0.240	0.0	0.001	PM
N3304-01DUP	-0.054	0.0	0.001	6/13/22
N3304-01MS	32.535	0.0	0.026	
N3304-01MSD	32.375	0.0	0.026	
N3304-02	0.559	0.0	0.001	
N3340-03	0.659	0.0	0.001	
CCV2	244.017	0.0	0.189	
CCB2	0.591	0.0	0.001	
N3304-04	-0.065	0.0	0.001	
N3304-015	0.243	0.0	0.001	
N3304-06	1.083	0.0	0.002	PM 6/13/22
N3214-03	2.309	0.0	0.003	
N3214-03RE	3.664	0.0	0.004	
CCV3	244.157	0.0	0.189	
CCB3	0.335	0.0	0.001	

N 23
Mean 64.969
SD 124.2735
CV% 191.28

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 13 10:37:50 2022

Mon Jun 13 13:17:34 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.3041	µg/l	6/13/2022 10:37:50	
5.OPPBCN	A	Total CN	P	4.1026	µg/l	6/13/2022 10:37:51	
10PPBCN	A	Total CN	P	9.6527	µg/l	6/13/2022 10:37:52	
50PPBCN	A	Total CN	P	49.2561	µg/l	6/13/2022 10:37:53	
100PPBCN	A	Total CN	P	98.7729	µg/l	6/13/2022 10:37:54	
250PPBCN	A	Total CN	P	255.1516	µg/l	6/13/2022 10:37:55	
500PPBCN	A	Total CN	P	497.7599	µg/l	6/13/2022 10:37:56	
ICV1	S	Total CN	P	94.085	µg/l	6/13/2022 12:59:40	
ICB1	S	Total CN	P	0.4692	µg/l	6/13/2022 12:59:41	
CCV1	S	Total CN	P	244.5484	µg/l	6/13/2022 12:59:44	
CCB1	S	Total CN	P	0.4033	µg/l	6/13/2022 12:59:46	
PB145491BL	S	Total CN	P	0.3413	µg/l	6/13/2022 12:59:47	
PB145491BS	S	Total CN	P	94.1608	µg/l	6/13/2022 13:07:11	
LOWPB145491	S	Total CN	P	9.8351	µg/l	6/13/2022 13:07:13	
HIGHPB145491	S	Total CN	P	487.7943	µg/l	6/13/2022 13:07:15	
N3304-01	S	Total CN	P	0.2398	µg/l	6/13/2022 13:07:17	
N3304-01DUP	S	Total CN	P	-0.0535	µg/l	6/13/2022 13:07:18	
N3304-01MS	S	Total CN	P	32.5352	µg/l	6/13/2022 13:07:19	
N3304-01MSD	S	Total CN	P	32.3749	µg/l	6/13/2022 13:07:20	
N3304-02	S	Total CN	P	0.559	µg/l	6/13/2022 13:14:47	
N3340-03	S	Total CN	P	0.6586	µg/l	6/13/2022 13:14:48	
CCV2	S	Total CN	P	244.0173	µg/l	6/13/2022 13:14:49	
CCB2	S	Total CN	P	0.5908	µg/l	6/13/2022 13:14:50	
N3304-04	S	Total CN	P	-0.0648	µg/l	6/13/2022 13:14:51	
N3304-05	S	Total CN	P	0.2431	µg/l	6/13/2022 13:14:52	
N3304-06	S	Total CN	P	1.0826	µg/l	6/13/2022 13:14:53	
N3214-03	S	Total CN	P	2.3095	µg/l	6/13/2022 13:14:54	
N3214-03RE	S	Total CN	P	3.664	µg/l	6/13/2022 13:14:55	
CCV3	S	Total CN	P	244.1574	µg/l	6/13/2022 13:14:56	
CCB3	S	Total CN	P	0.3348	µg/l	6/13/2022 13:17:34	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : DM

Instrument ID : Konelab

6/13/2022 11:02


Test Total CN

Accepted 6/13/2022 11:02

Factor 1297
Bias 0.001

Coeff. of det. 0.999831

Errors

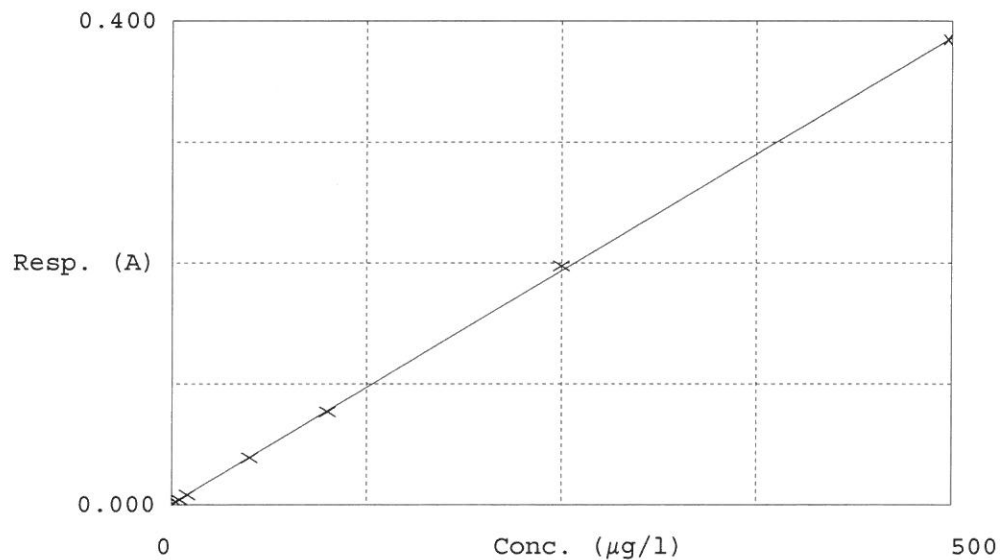

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.3041	0.0000	
2	5.0PPBCN	0.004	4.1026	5.0000	-17.9
3	10PPBCN	0.008	9.6527	10.0000	-3.5
4	50PPBCN	0.039	49.2561	50.0000	
5	100PPBCN	0.077	98.7729	100.0000	-1.5
6	250PPBCN	0.198	255.1516	250.0000	-1.2
7	500PPBCN	0.385	497.7599	500.0000	2.1

-0.4

DM

6/13/22