

LB 122566

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

10/21/2022 12:53 Reviewed by : 17 Instrument ID : Konelab

Test: Phenolics-

Sample Id	^{W/L} Result	Dil. 1 +	Response	Errors
ICV1	0.973	0.0	0.110	
ICB1	-0.018	0.0	0.007	
CCV1	1.005	0.0	0.113	
CCB1	-0.019	0.0	0.007	
PB148488BL	-0.019	0.0	0.007	
PB148488BS	0.972	0.0	0.109	
N4788-27	1.451	0.0	0.159	
N4955-10	0.017	0.0	0.010	
N4955-11	0.052	0.0	0.014	
CCV2	0.969	0.0	0.109	
CCB2	-0.019	0.0	0.007	
N	11			
Mean	0.488			
SD	0.5774			
CV%	118.36			

Aquakem v. 7.2AQ1

Results from time period:

Fri Oct 21 12:30:16 2022

Fri Oct 21 12:38:07 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0008	mg/l	10/21/2022 10:29:51	
0.05PPM	A	Phenolics-	P	0.0572	mg/l	10/21/2022 10:29:52	
0.1PPM	A	Phenolics-	P	0.1058	mg/l	10/21/2022 10:29:53	
0.25PPM	A	Phenolics-	P	0.2517	mg/l	10/21/2022 10:29:54	
0.50PPM	A	Phenolics-	P	0.4987	mg/l	10/21/2022 10:29:55	
1.0PPM	A	Phenolics-	P	0.9724	mg/l	10/21/2022 10:29:56	
2.0PPM	A	Phenolics-	P	2.0134	mg/l	10/21/2022 10:29:57	
ICV1	S	Phenolics-	P	0.9733	mg/l	10/21/2022 12:30:17	
ICB1	S	Phenolics-	P	-0.0176	mg/l	10/21/2022 12:30:18	
CCV1	S	Phenolics-	P	1.0048	mg/l	10/21/2022 12:30:21	
CCB1	S	Phenolics-	P	-0.0189	mg/l	10/21/2022 12:30:23	
PB148488BL	S	Phenolics-	P	-0.0189	mg/l	10/21/2022 12:30:25	
PB148488BS	S	Phenolics-	P	0.972	mg/l	10/21/2022 12:30:27	
N4788-27	S	Phenolics-	P	1.451	mg/l	10/21/2022 12:37:59	
N4955-10	S	Phenolics-	P	0.0174	mg/l	10/21/2022 12:38:00	
N4955-11	S	Phenolics-	P	0.0522	mg/l	10/21/2022 12:38:03	
CCV2	S	Phenolics-	P	0.9692	mg/l	10/21/2022 12:38:05	
CCB2	S	Phenolics-	P	-0.0187	mg/l	10/21/2022 12:38:06	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

10/21/2022 10:30


Test Phenolics-

Accepted 10/21/2022 10:30

Factor 9.625
Bias 0.008

Coeff. of det. 0.999672

Errors

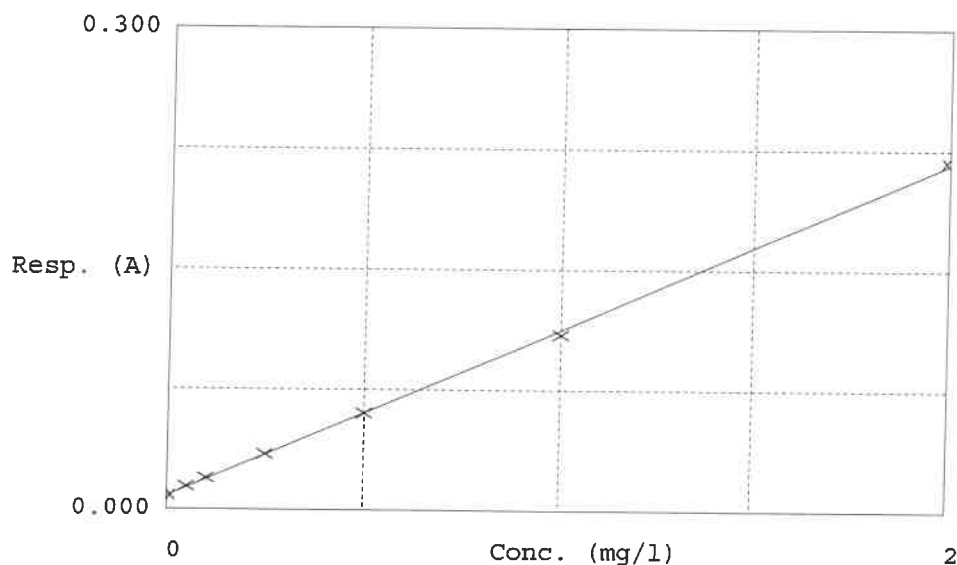

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.009	0.0008	0.0000	-
2	Phenol-2	0.014	0.0572	0.0500	14.4
3	Phenol-2	0.019	0.1058	0.1000	5.8
4	Phenol-2	0.035	0.2517	0.2500	0.7
5	Phenol-2	0.060	0.4987	0.5000	-0.3
6	Phenol-2	0.110	0.9724	1.0000	-2.8
7	Phenol-2	0.218	2.0134	2.0000	0.7

10/21/22