

Clear table

Instrument ID: IC-2										Analyst : IZ		Method: 300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-01-19_	1/19/23 11:00		IZ/MA		
STD2	0.4880	0.6840	0.7060	2.3300	0.5760	1.0560	3.4740	0.0000_2023-01-19_	1/19/23 11:31		IZ/MA		
STD3	0.7760	1.2150	1.2130	4.0420	1.0070	2.0000	6.0020	0.0000_2023-01-19_	1/19/23 12:01		IZ/MA		
STD4	0.9450	1.5030	1.5180	5.0520	1.2780	2.5430	7.4510	0.0000_2023-01-19_	1/19/23 12:32		IZ/MA		
STD5	1.8550	2.8760	2.8370	9.5070	2.3720	4.8860	14.5380	0.0000_2023-01-19_	1/19/23 13:02		IZ/MA		
STD6	3.9270	5.9350	5.9150	19.6950	4.9230	9.9270	29.5160	0.0000_2023-01-19_	1/19/23 13:33		IZ/MA		
STD7	5.0990	7.5870	7.6110	25.3740	6.3440	12.5880	38.0180	0.0000_2023-01-19_	1/19/23 14:04		IZ/MA		
ICV	1.8290	2.9990	3.0090	9.9010	2.4740	4.7390	14.6300	0.0000_2023-01-19_	1/19/23 15:07		IZ/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-01-19_	1/19/23 15:38		IZ/MA		
CCV	2.0300	2.9170	2.8790	9.7190	2.4030	5.2600	14.2310	0.0000_2023-02-14_	2/14/23 10:02		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-02-14_	2/14/23 10:38		IZ/MA		
LB124093BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-02-14_	2/14/23 11:09		IZ/MA		
LB124093BSW	1.8800	2.9570	2.8820	9.7900	2.4380	5.0020	14.4420	0.0000_2023-02-14_	2/14/23 11:41		IZ/MA		
O1544-01	0.0000	0.3390	0.0000	0.0000	0.3460	0.4800	1.2200	0.0000_2023-02-14_	2/14/23 12:26		IZ/MA		
O1544-01MS	1.9670	3.0570	2.8260	9.6090	2.6200	5.0460	14.4410	0.0000_2023-02-14_	2/14/23 12:58		IZ/MA		
O1544-01MSD	1.9450	3.0640	2.8430	9.6120	2.6220	4.8570	14.4390	0.0000_2023-02-14_	2/14/23 15:47		IZ/MA		
O1553-05	0.6900	129.4960	0.0000	0.0000	1.1730	0.0000	3.5290	0.0000_2023-02-14_	2/14/23 17:22		IZ/MA		
CCV	2.0040	2.9920	3.0350	9.9220	2.4640	6.2110	14.6240	0.0000_2023-02-14_	2/14/23 17:54		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-02-14_	2/14/23 18:26		IZ/MA		

Report date: 2/15/2023 2:54:31 PM
Printed by: wet


Ident: CCV
Analysis from: 2/14/2023 10:02:29 AM
File: _2023-02-14_

Last save: 2/14/2023 10:35:21 AM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33288

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

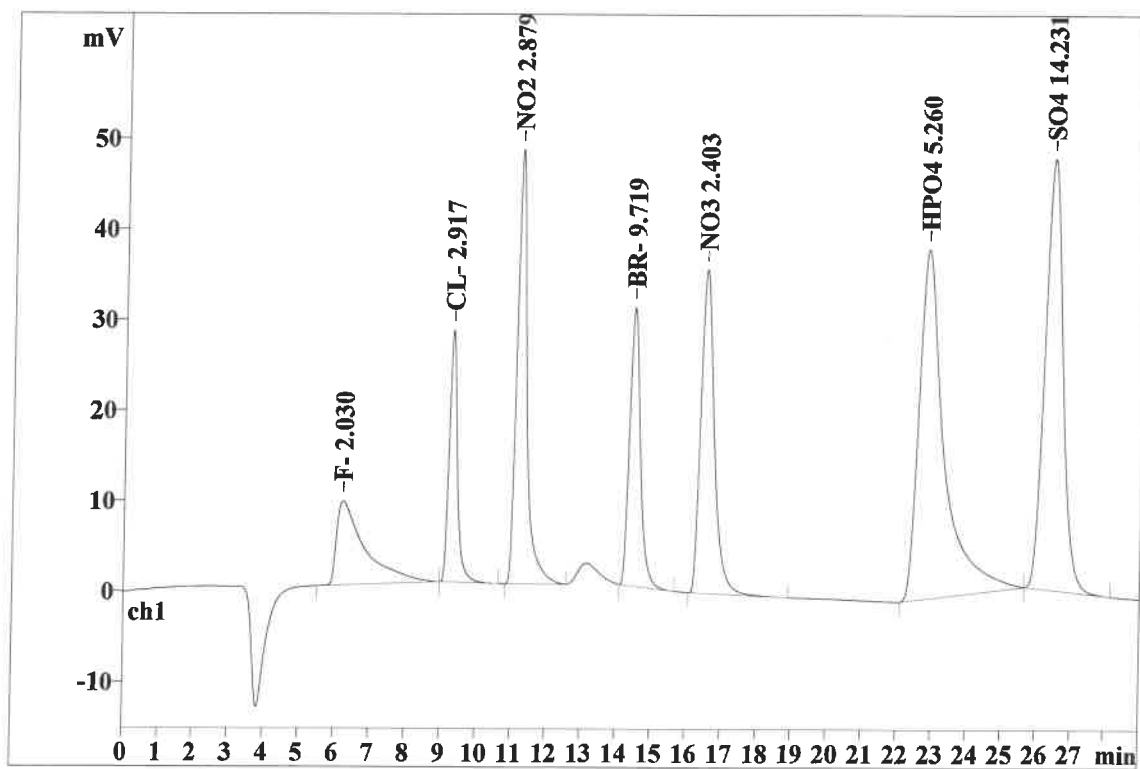

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.22	0.714	9.26	3.89	512.084	7.11
2	9.28	0.234	27.84	11.71	448.067	6.22
3	11.18	0.286	47.96	20.18	973.580	13.51
4	14.46	0.323	30.75	12.94	660.668	9.17
5	16.49	0.390	35.74	15.04	942.364	13.08
6	22.80	0.662	38.57	16.23	1950.460	27.07
7	26.39	0.552	47.58	20.01	1717.290	23.84
7	29.00	0.451	237.70	100.00	7204.513	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/15/2023 2:54:40 PM
Printed by: wet


Ident: CCB
Analysis from: 2/14/2023 10:38:03 AM
File: _2023-02-14_

Last save: 2/14/2023 11:07:04 AM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33289

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

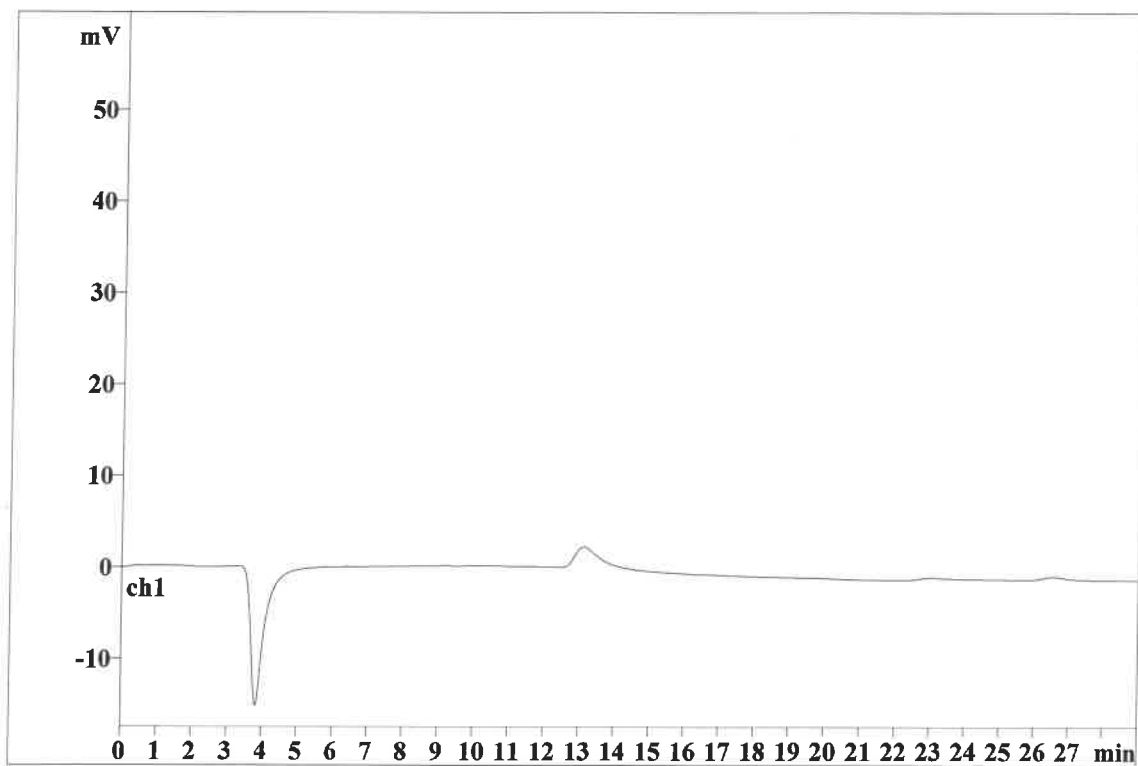

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/15/2023 2:54:47 PM
Printed by: wet


Ident: LB124093BLW
Analysis from: 2/14/2023 11:09:41 AM
File: _2023-02-14_

Last save: 2/15/2023 2:54:23 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33290

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

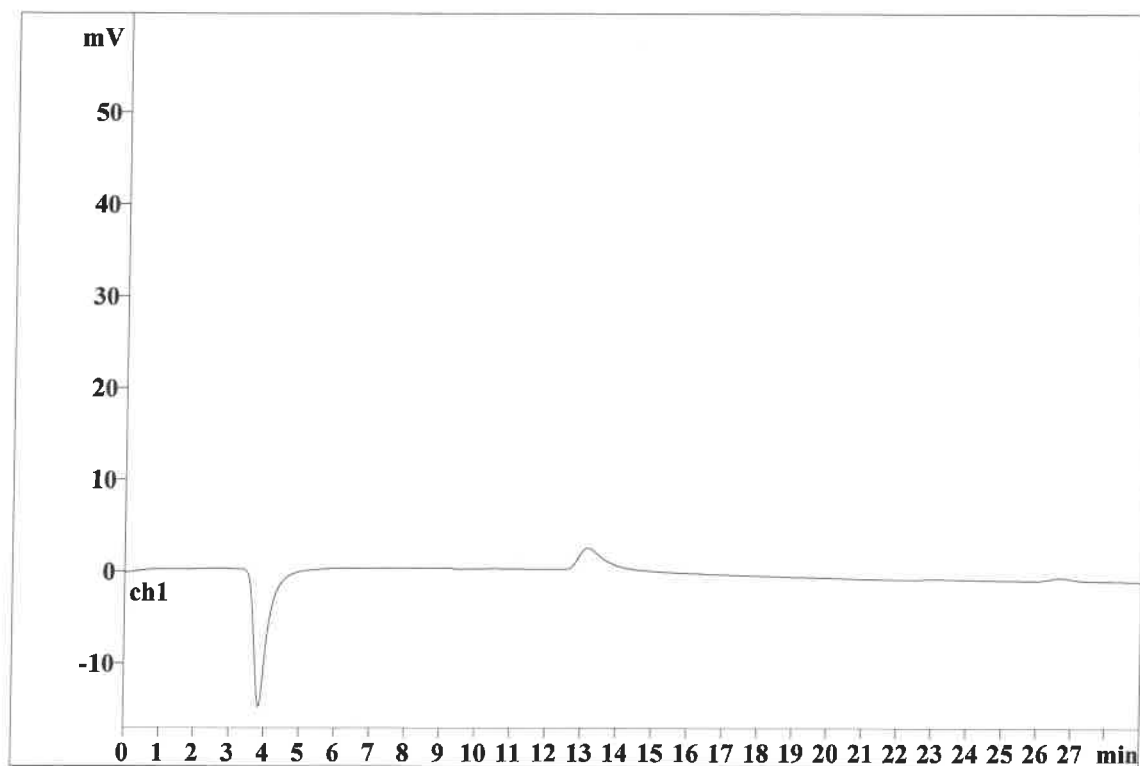

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/15/2023 2:54:55 PM
Printed by: wet


Ident: LB124093BSW
Analysis from: 2/14/2023 11:41:19 AM
File: _2023-02-14_

Last save: 2/15/2023 2:54:23 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33291

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

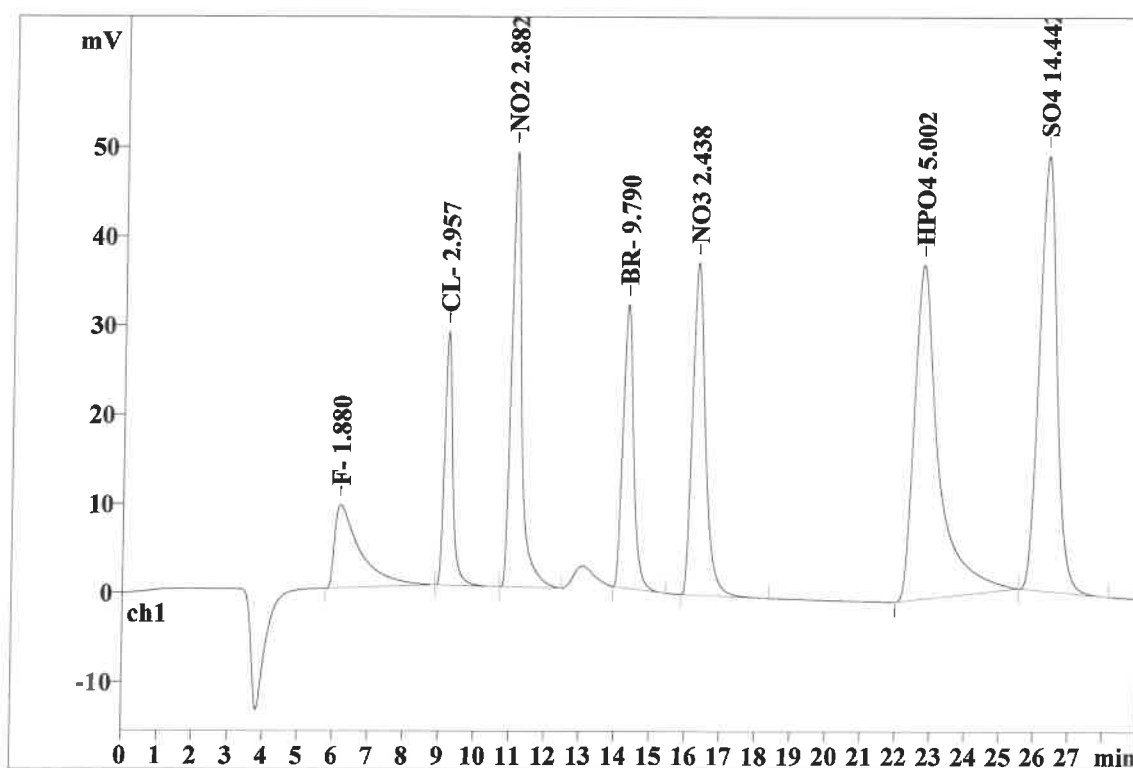

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.17	0.676	9.32	3.85	470.282	6.61
2	9.19	0.230	28.50	11.77	454.449	6.39
3	11.07	0.281	48.80	20.16	974.690	13.70
4	14.28	0.315	31.83	13.15	665.903	9.36
5	16.27	0.380	37.28	15.40	956.819	13.45
6	22.70	0.645	37.52	15.50	1846.196	25.96
7	26.28	0.547	48.76	20.15	1744.566	24.53
7	29.00	0.439	242.00	100.00	7112.905	100.00

Report date: 2/15/2023 2:55:07 PM
Printed by: wet


Ident: 01544-01
Analysis from: 2/14/2023 12:26:39 PM
File: _2023-02-14_

Last save: 2/14/2023 12:55:40 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33292

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

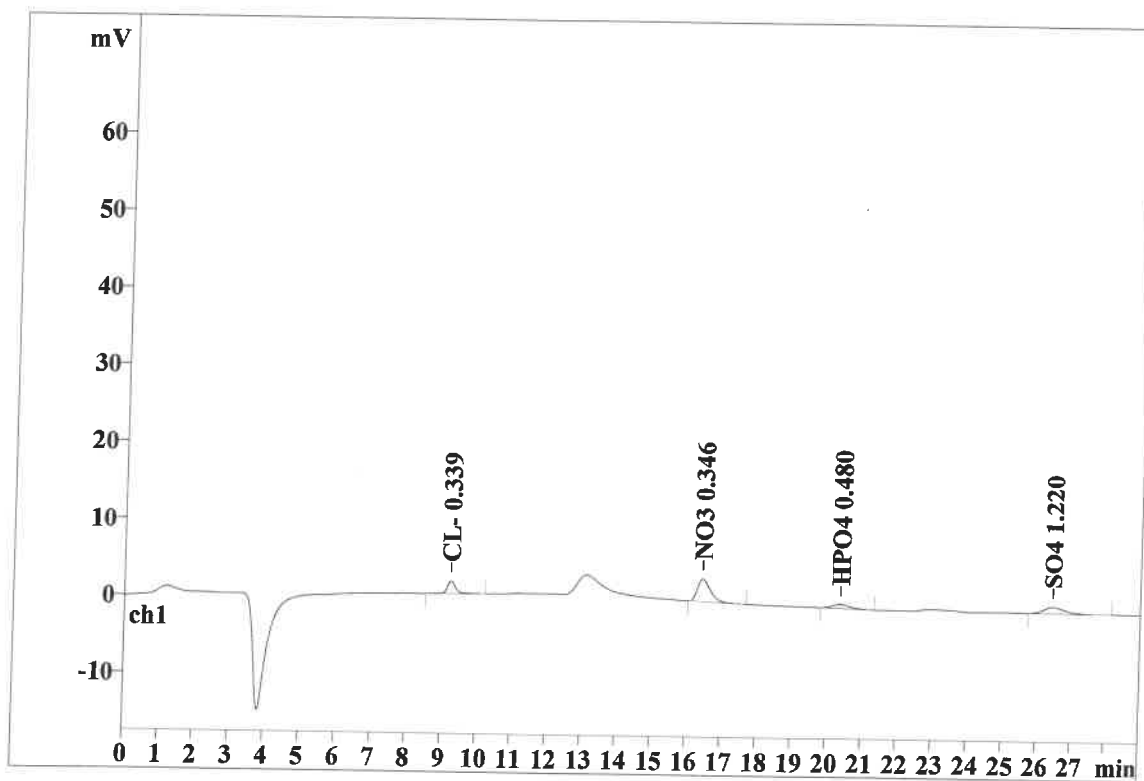

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.24	0.238	1.60	26.97	27.890	17.53
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.44	0.393	2.94	49.69	76.537	48.10
6	20.37	0.533	0.53	8.95	18.245	11.47
7	26.44	0.647	0.85	14.27	36.440	22.90
7	29.00	0.259	5.92	99.88	159.113	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/15/2023 2:55:14 PM
Printed by: wet


Ident: 01544-01MS
Analysis from: 2/14/2023 12:58:18 PM
File: _2023-02-14_

Last save: 2/14/2023 3:02:53 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33293

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

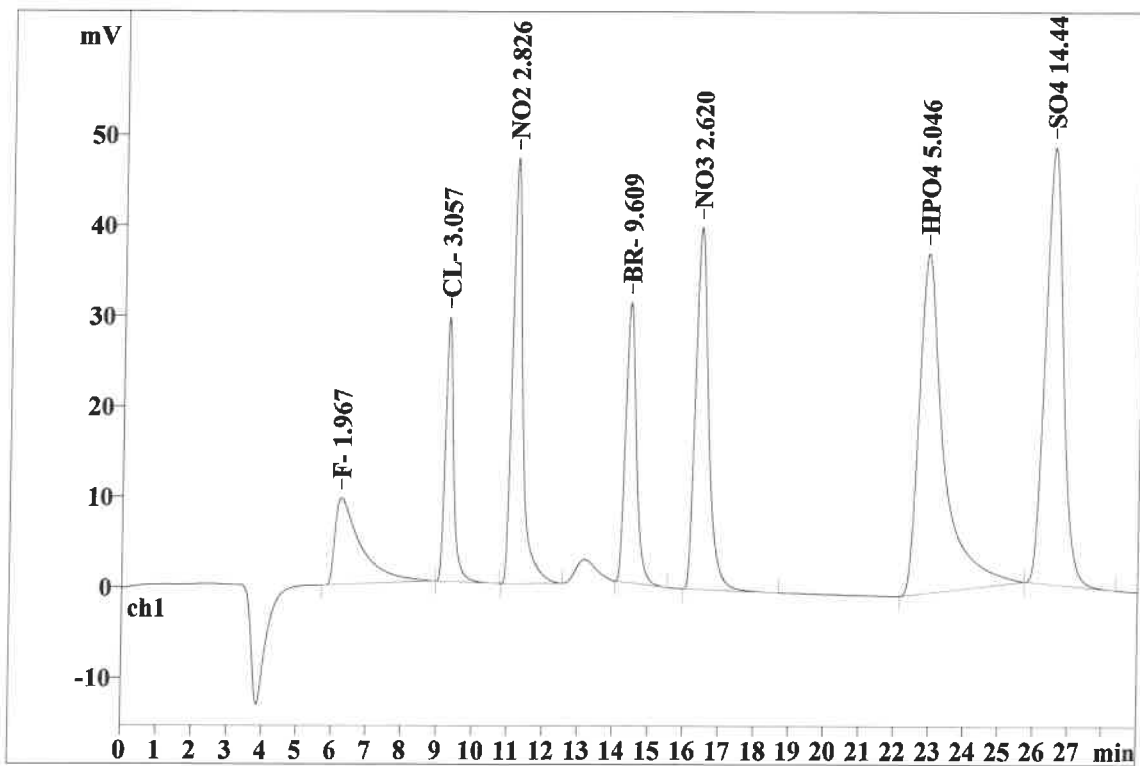

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.23	0.694	9.60	3.95	494.623	6.86
2	9.27	0.233	29.21	12.04	470.830	6.53
3	11.15	0.285	47.04	19.38	953.842	13.22
4	14.41	0.317	30.97	12.76	652.594	9.05
5	16.39	0.383	40.02	16.49	1033.533	14.33
6	22.87	0.651	37.55	15.47	1863.845	25.84
7	26.48	0.552	48.26	19.89	1744.455	24.18
7	29.00	0.445	242.64	100.00	7213.723	100.00

Report date: 2/15/2023 2:55:35 PM
Printed by: wet


Ident: O1544-01MSD
Analysis from: 2/14/2023 3:47:25 PM
File: _2023-02-14_

Last save: 2/15/2023 2:55:33 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33298

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

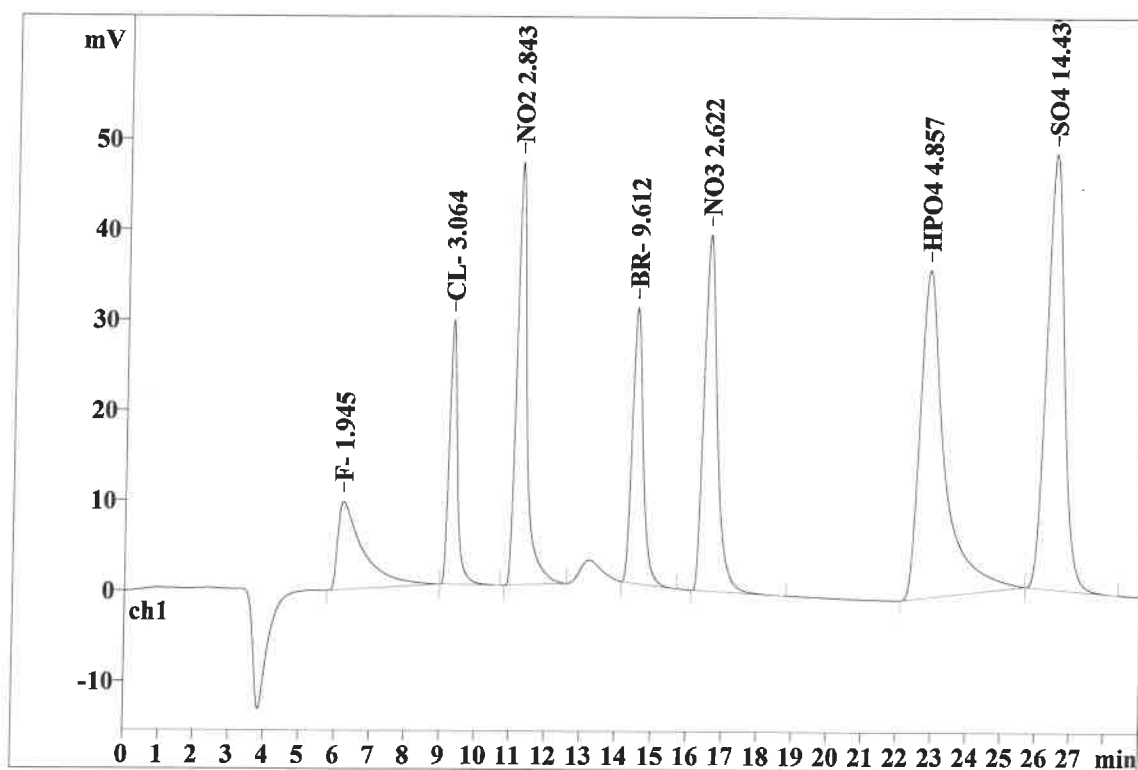

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.19	0.655	9.77	4.07	488.302	6.84
2	9.28	0.233	29.27	12.18	472.026	6.61
3	11.19	0.288	46.77	19.47	960.343	13.45
4	14.49	0.322	30.53	12.71	652.768	9.14
5	16.52	0.390	39.42	16.41	1034.420	14.49
6	22.82	0.648	36.28	15.10	1787.503	25.04
7	26.42	0.553	48.21	20.07	1744.236	24.43
7	29.00	0.441	240.27	100.00	7139.598	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/15/2023 2:56:02 PM
Printed by: wet


Ident: O1553-05
Analysis from: 2/14/2023 5:22:55 PM
File: _2023-02-14_

Last save: 2/15/2023 2:55:52 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33301

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

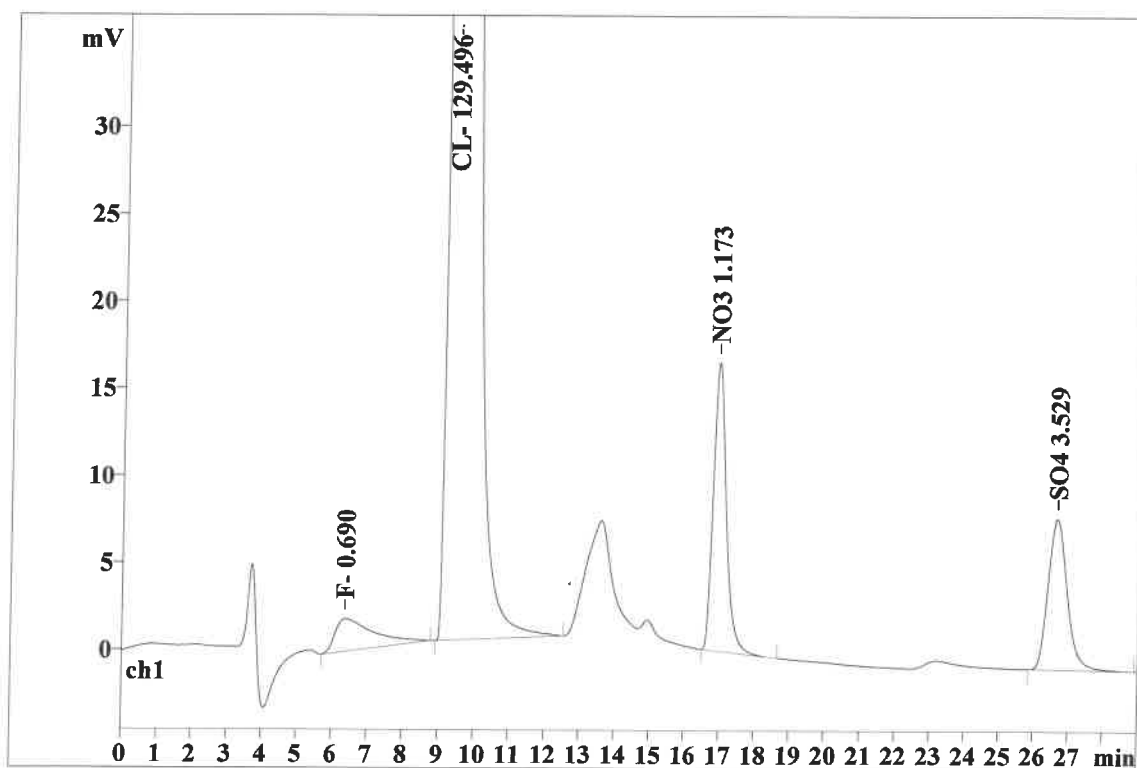

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.37	1.085	1.86	0.18	139.355	0.63
2	9.40	0.300	1006.64	97.38	21075.081	95.91
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.92	0.384	16.55	1.60	424.507	1.93
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.65	0.581	8.66	0.84	334.737	1.52
7	29.00	0.336	1033.71	100.00	21973.680	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/15/2023 2:56:09 PM
Printed by: wet


Ident: CCV
Analysis from: 2/14/2023 5:54:38 PM
File: _2023-02-14_

Last save: 2/15/2023 9:19:08 AM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33302

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

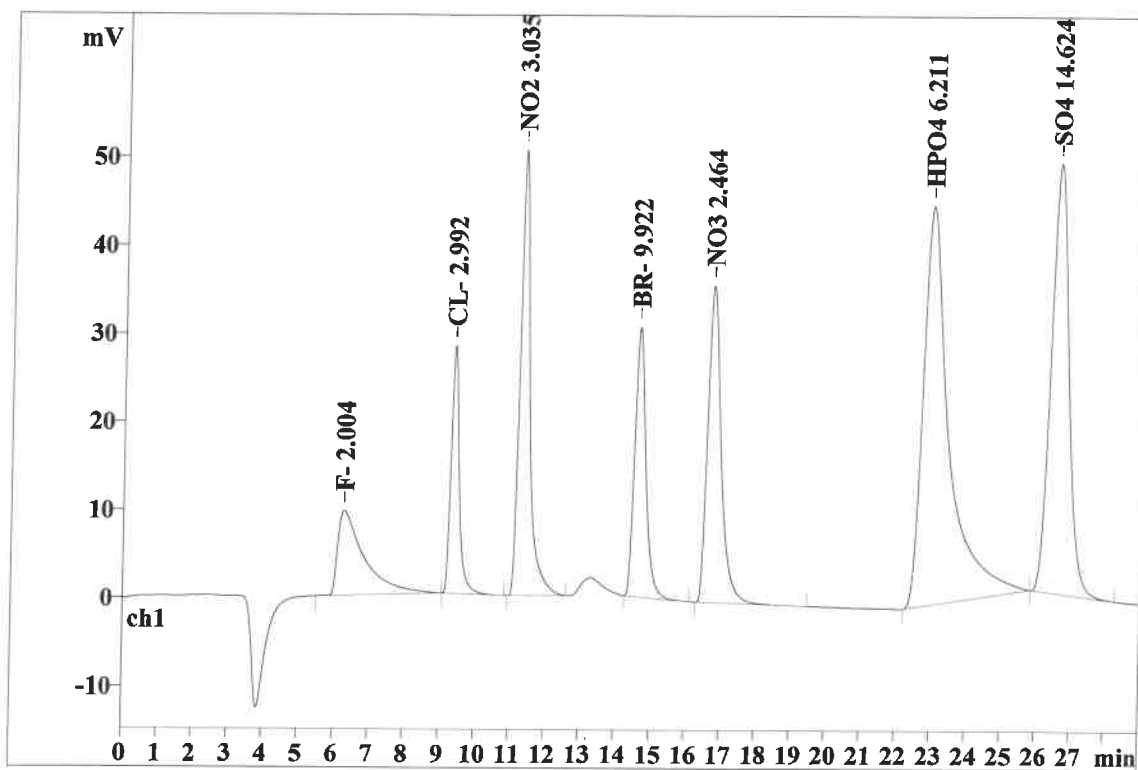

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.27	0.706	9.60	3.86	504.790	6.52
2	9.38	0.237	28.11	11.31	460.218	5.94
3	11.31	0.289	50.48	20.31	1031.679	13.32
4	14.63	0.332	30.53	12.29	675.705	8.73
5	16.71	0.399	35.91	14.45	967.808	12.50
6	22.95	0.673	45.20	18.19	2334.944	30.15
7	26.58	0.555	48.69	19.59	1768.090	22.83
7	29.00	0.456	248.53	100.00	7743.234	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/15/2023 2:56:17 PM
Printed by: wet


Ident: CCB
Analysis from: 2/14/2023 6:26:18 PM
File: _2023-02-14_

Last save: 2/14/2023 6:55:18 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33303

Last save: 2/10/2023 11:57

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

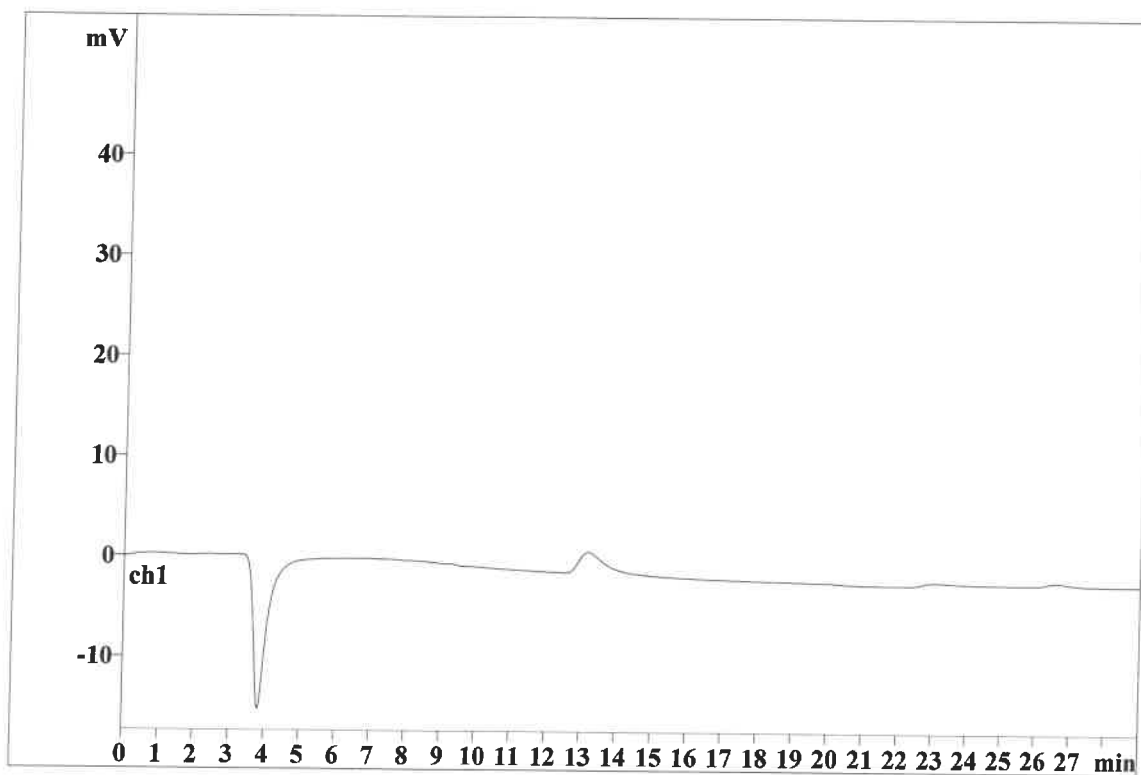

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD