

6127071

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

8/30/2023 8:00

Reviewed by : PM

Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.067	0.0	0.114	
ICB1	0.011	0.0	0.009	
CCV1	1.006	0.0	0.108	
CCB1	0.006	0.0	0.008	
PB155112BL	0.014	0.0	0.009	
PB155112BS	1.067	0.0	0.114	
O4152-01	-0.441	0.0	-0.036	
O4152-01DUP	-0.820	0.0	-0.074	
O4152-01MS	1.224	0.0	0.130	
O4152-01MSD	1.019	0.0	0.109	
CCV2	1.017	0.0	0.109	
CCB2	0.014	0.0	0.009	

N	12
Mean	0.432
SD	0.7062
CV%	163.48

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 29 16:31:07 2023

Tue Aug 29 18:38:32 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0064	mg/l	8/29/2023 16:31:07	
0.05PPM	A	Phenolics-	P	0.0615	mg/l	8/29/2023 16:31:08	
0.1PPM	A	Phenolics-	P	0.0919	mg/l	8/29/2023 16:31:09	
0.25PPM	A	Phenolics-	P	0.2491	mg/l	8/29/2023 16:31:10	
0.50PPM	A	Phenolics-	P	0.5014	mg/l	8/29/2023 16:31:11	
1.0PPM	A	Phenolics-	P	0.9795	mg/l	8/29/2023 16:31:12	
2.0PPM	A	Phenolics-	P	2.0101	mg/l	8/29/2023 16:31:13	
ICV1	S	Phenolics-	P	1.0666	mg/l	8/29/2023 18:24:32	
ICB1	S	Phenolics-	P	0.0114	mg/l	8/29/2023 18:24:34	
CCV1	S	Phenolics-	P	1.0059	mg/l	8/29/2023 18:24:36	
CCB1	S	Phenolics-	P	0.0064	mg/l	8/29/2023 18:24:38	
PB155112BL	S	Phenolics-	P	0.0139	mg/l	8/29/2023 18:24:40	
PB155112BS	S	Phenolics-	P	1.0671	mg/l	8/29/2023 18:24:42	
O4152-01	S	Phenolics-	P	-0.4408	mg/l	8/29/2023 18:34:34	
O4152-01DUP	S	Phenolics-	P	-0.8202	mg/l	8/29/2023 18:34:36	
O4152-01MS	S	Phenolics-	P	1.2236	mg/l	8/29/2023 18:34:38	
O4152-01MSD	S	Phenolics-	P	1.0193	mg/l	8/29/2023 18:34:43	
CCV2	S	Phenolics-	P	1.0168	mg/l	8/29/2023 18:34:44	
CCB2	S	Phenolics-	P	0.0139	mg/l	8/29/2023 18:38:31	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

8/29/2023 17:52

Test Phenolics-


Accepted 8/29/2023 17:52

Factor 10.01

Bias 0.008

Coeff. of det. 0.999758

Errors

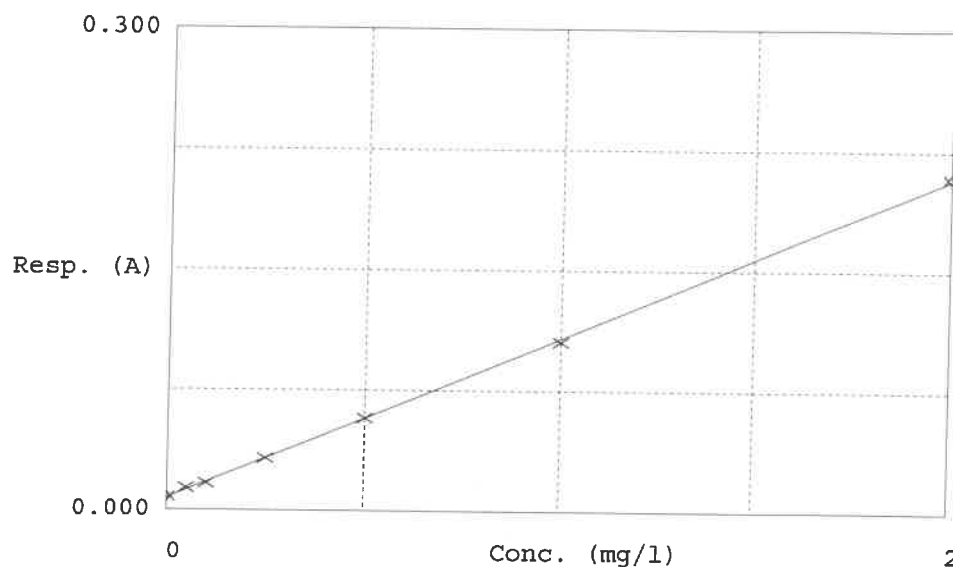

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.008	0.0064	0.0000	-
2	Phenol-2	0.014	0.0615	0.0500	23.0
3	Phenol-2	0.017	0.0919	0.1000	-8.1
4	Phenol-2	0.032	0.2491	0.2500	-0.4
5	Phenol-2	0.058	0.5014	0.5000	0.3
6	Phenol-2	0.105	0.9795	1.0000	-2.1
7	Phenol-2	0.208	2.0101	2.0000	0.5

08/29/23
RM