

LB127518

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

9/28/2023 13:40

Reviewed by : 12

Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.976	0.0	0.123	
ICB1	0.003	0.0	0.018	
CCV1	1.010	0.0	0.127	
CCB1	0.004	0.0	0.018	
PB155940BL	0.004	0.0	0.018	
12 PB155490BL 940BS	0.985	0.0	0.124	
940BS O4349-25	2.199	0.0	0.256	Test limit high
940BS CCB2	1.008	0.0	0.127	
	0.001	0.0	0.017	
O4349-25DLX2	1.096	0.0	0.136	
CCV3	1.015	0.0	0.128	
CCB3	0.002	0.0	0.018	

N 12
Mean 0.692
SD 0.6929
CV% 100.15

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 28 11:55:44 2023

Thu Sep 28 13:34:46 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0031	mg/l	9/28/2023 12:28:52	
0.05PPM	A	Phenolics-	P	0.0526	mg/l	9/28/2023 12:28:53	
0.1PPM	A	Phenolics-	P	0.1011	mg/l	9/28/2023 12:28:54	
0.25PPM	A	Phenolics-	P	0.2507	mg/l	9/28/2023 12:28:55	
0.50PPM	A	Phenolics-	P	0.4991	mg/l	9/28/2023 12:28:56	
1.0PPM	A	Phenolics-	P	0.9866	mg/l	9/28/2023 12:28:57	
2.0PPM	A	Phenolics-	P	2.0067	mg/l	9/28/2023 12:28:58	
ICV1	S	Phenolics-	P	0.9763	mg/l	9/28/2023 12:51:31	
ICB1	S	Phenolics-	P	0.0026	mg/l	9/28/2023 12:51:33	
CCV1	S	Phenolics-	P	1.0099	mg/l	9/28/2023 12:51:36	
CCB1	S	Phenolics-	P	0.0045	mg/l	9/28/2023 12:51:38	
PB155940BL	S	Phenolics-	P	0.0041	mg/l	9/28/2023 12:51:40	
PB155940BS	S	Phenolics-	P	0.9847	mg/l	9/28/2023 12:51:42	
O4349-25	S	Phenolics-	P	2.1992	mg/l	9/28/2023 12:58:17	
CCV2	S	Phenolics-	P	1.0076	mg/l	9/28/2023 12:58:21	
CCB2	S	Phenolics-	P	0.0008	mg/l	9/28/2023 12:58:23	
O4349-25DLX2	S	Phenolics-	P	1.0962	mg/l	9/28/2023 13:34:42	
CCV3	S	Phenolics-	P	1.0145	mg/l	9/28/2023 13:34:43	
CCB3	S	Phenolics-	P	0.002	mg/l	9/28/2023 13:34:46	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

9/28/2023 12:30

Test Phenolics-


Accepted 9/28/2023 12:29

Factor 9.213

Bias 0.017

Coeff. of det. 0.999923

Errors

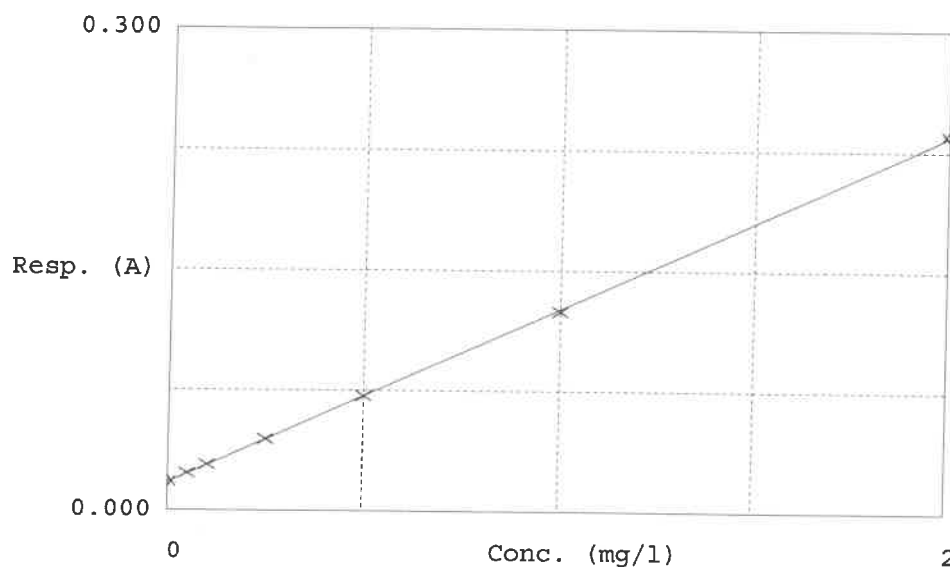

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.018	0.0031	0.0000	-
2	Phenol-2	0.023	0.0526	0.0500	5.2
3	Phenol-2	0.028	0.1011	0.1000	1.1
4	Phenol-2	0.045	0.2507	0.2500	0.3
5	Phenol-2	0.072	0.4991	0.5000	-0.2
6	Phenol-2	0.124	0.9866	1.0000	-1.3
7	Phenol-2	0.235	2.0067	2.0000	0.3

12
9/28/23