

66129262

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

1/26/2024 11:09

Test: Total CN

Sample Id	<i>mark</i> Result	Dil. 1 +	Response	Errors
ICV1	95.307	0.0	0.072	
ICB1	1.162	0.0	0.001	
CCV1	241.664	0.0	0.182	
CCB1	0.696	0.0	0.001	
PB158614BL	0.499	0.0	0.001	
P1240-03	1.081	0.0	0.001	
P1240-03DUP	1.098	0.0	0.001	
P1240-06	1.574	0.0	0.001	
P1240-09	0.899	0.0	0.001	
P1243-02	1.208	0.0	0.001	
P1243-04	0.838	0.0	0.001	
P1246-03	0.683	0.0	0.001	
CCV2	243.218	0.0	0.183	
CCB2	0.973	0.0	0.001	

N 14
Mean 42.207
SD 88.4529
CV% 209.57

Aquakem v. 7.2AQ1

Results from time period:

Fri Jan 26 09:49:28 2024

Fri Jan 26 10:49:35 2024

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.8576	µg/l	1/26/2024 10:06:44	
5.0PPBCN	A	Total CN	P	5.4991	µg/l	1/26/2024 10:06:45	
10PPBCN	A	Total CN	P	10.3151	µg/l	1/26/2024 10:06:46	
50PPBCN	A	Total CN	P	48.4422	µg/l	1/26/2024 10:06:47	
100PPBCN	A	Total CN	P	99.5148	µg/l	1/26/2024 10:06:48	
250PPBCN	A	Total CN	P	250.2592	µg/l	1/26/2024 10:06:49	
500PPBCN	A	Total CN	P	500.1119	µg/l	1/26/2024 10:06:50	
ICV1	S	Total CN	P	95.3073	µg/l	1/26/2024 10:35:16	
ICB1	S	Total CN	P	1.1617	µg/l	1/26/2024 10:35:18	
CCV1	S	Total CN	P	241.6637	µg/l	1/26/2024 10:35:21	
CCB1	S	Total CN	P	0.6955	µg/l	1/26/2024 10:35:22	
PB158614BL	S	Total CN	P	0.4985	µg/l	1/26/2024 10:35:24	
P1240-03	S	Total CN	P	1.0814	µg/l	1/26/2024 10:42:48	
P1240-03DUP	S	Total CN	P	1.0982	µg/l	1/26/2024 10:42:50	
P1240-06	S	Total CN	P	1.5738	µg/l	1/26/2024 10:42:51	
P1240-09	S	Total CN	P	0.8985	µg/l	1/26/2024 10:42:52	
P1243-02	S	Total CN	P	1.2078	µg/l	1/26/2024 10:42:53	
P1243-04	S	Total CN	P	0.8378	µg/l	1/26/2024 10:42:54	
P1246-03	S	Total CN	P	0.6828	µg/l	1/26/2024 10:42:55	
CCV2	S	Total CN	P	243.2177	µg/l	1/26/2024 10:49:31	
CCB2	S	Total CN	P	0.9734	µg/l	1/26/2024 10:49:35	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

1/26/2024 10:08


Test Total CN

Accepted 1/26/2024 10:08

Factor 1332
Bias 0

Coeff. of det. 0.999981

Errors

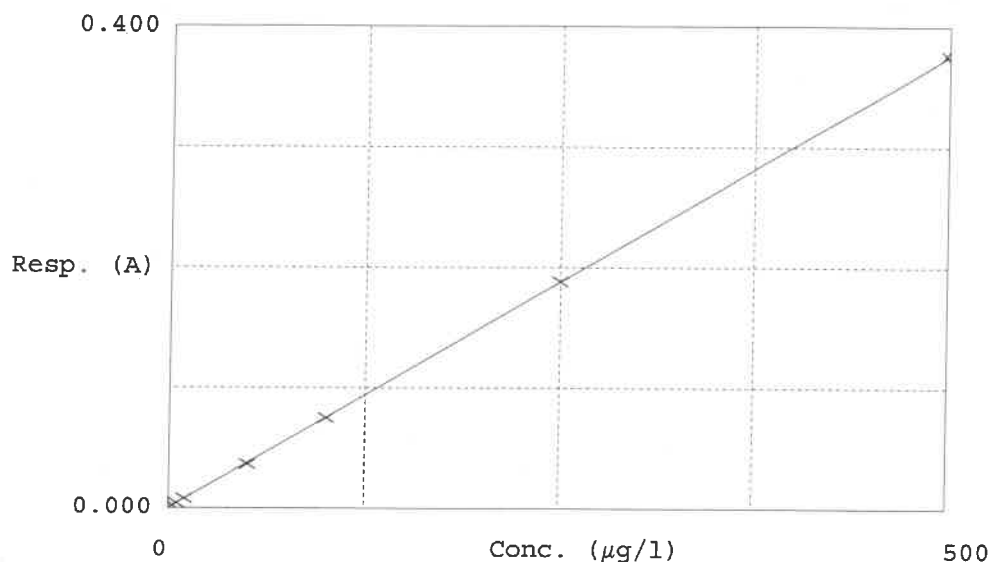

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.8576	0.0000	10.0
2	5.0PPBCN	0.004	5.4991	5.0000	3.2
3	10PPBCN	0.008	10.3151	10.0000	-3.1
4	50PPBCN	0.037	48.4422	50.0000	-0.5
5	100PPBCN	0.075	99.5148	100.0000	0.1
6	250PPBCN	0.188	250.2592	250.0000	0.0
7	500PPBCN	0.376	500.1119	500.0000	

01/26/2024
RM