

6130874

=====

Test results	Aquakem 7.2AQ1	Page: 1
--------------	----------------	---------

=====

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

5/22/2024 10:22 Reviewed by : RM Instrument ID : Konelab

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors

ICV1	92.918	0.0	0.062	
ICB1	1.402	0.0	0.002	
CCV1	246.416	0.0	0.162	
CCB1	1.561	0.0	0.002	
PB161019BL	1.226	0.0	0.002	
P2531-04	1.336	0.0	0.002	
P2531-04DUP	1.237	0.0	0.002	
P2538-03	1.425	0.0	0.002	
P2539-04	1.233	0.0	0.002	
P2539-08	1.489	0.0	0.002	
P2556-02	1.350	0.0	0.002	
P2558-02	1.320	0.0	0.002	
P2563-01	1.339	0.0	0.002	
PB161020BL	1.422	0.0	0.002	
CCV2	246.310	0.0	0.162	
CCB2	1.177	0.0	0.002	
P2538-04	1.243	0.0	0.002	
P2538-04DUP	1.359	0.0	0.002	
P2541-01	1.074	0.0	0.002	
P2563-03	1.511	0.0	0.002	
CCV3	254.558	0.0	0.168	
CCB3	1.484	0.0	0.002	
N	22			
Mean	39.290			
SD	87.5305			
CV%	222.78			

Aquakem v. 7.2AQ1

Results from time period:

Wed May 22 08:39:24 2024

Wed May 22 10:21:40 2024

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	1.2464	µg/l	5/22/2024 9:37:23	
5.0PPBCN	A	Total CN	P	5.7593	µg/l	5/22/2024 9:37:24	
10PPBCN	A	Total CN	P	9.4359	µg/l	5/22/2024 9:37:25	
50PPBCN	A	Total CN	P	47.8745	µg/l	5/22/2024 9:37:26	
100PPBCN	A	Total CN	P	97.9471	µg/l	5/22/2024 9:37:27	
250PPBCN	A	Total CN	P	254.2198	µg/l	5/22/2024 9:37:28	
500PPBCN	A	Total CN	P	498.5169	µg/l	5/22/2024 9:37:29	
ICV1	S	Total CN	P	92.9184	µg/l	5/22/2024 10:03:18	
ICB1	S	Total CN	P	1.4016	µg/l	5/22/2024 10:03:20	
CCV1	S	Total CN	P	246.4156	µg/l	5/22/2024 10:03:23	
CCB1	S	Total CN	P	1.5608	µg/l	5/22/2024 10:03:24	
PB161019BL	S	Total CN	P	1.2259	µg/l	5/22/2024 10:03:26	
P2531-04	S	Total CN	P	1.3365	µg/l	5/22/2024 10:03:28	
P2531-04DUP	S	Total CN	P	1.2371	µg/l	5/22/2024 10:10:53	
P2538-03	S	Total CN	P	1.4252	µg/l	5/22/2024 10:10:54	
P2539-04	S	Total CN	P	1.2334	µg/l	5/22/2024 10:10:55	
P2539-08	S	Total CN	P	1.4892	µg/l	5/22/2024 10:10:56	
P2556-02	S	Total CN	P	1.35	µg/l	5/22/2024 10:10:57	
P2558-02	S	Total CN	P	1.3201	µg/l	5/22/2024 10:10:58	
P2563-01	S	Total CN	P	1.3391	µg/l	5/22/2024 10:10:59	
PB161020BL	S	Total CN	P	1.4221	µg/l	5/22/2024 10:11:00	
CCV2	S	Total CN	P	246.3099	µg/l	5/22/2024 10:11:03	
CCB2	S	Total CN	P	1.1766	µg/l	5/22/2024 10:15:40	
P2538-04	S	Total CN	P	1.243	µg/l	5/22/2024 10:15:41	
P2538-04DUP	S	Total CN	P	1.3587	µg/l	5/22/2024 10:15:42	
P2541-01	S	Total CN	P	1.0743	µg/l	5/22/2024 10:15:43	
P2563-03	S	Total CN	P	1.5107	µg/l	5/22/2024 10:15:44	
CCV3	S	Total CN	P	254.5578	µg/l	5/22/2024 10:21:39	
CCB3	S	Total CN	P	1.4842	µg/l	5/22/2024 10:21:40	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

5/22/2024 9:37


Test Total CN

Accepted 5/22/2024 9:37

Factor 1528
Bias 0.001

Coeff. of det. 0.999848

Errors

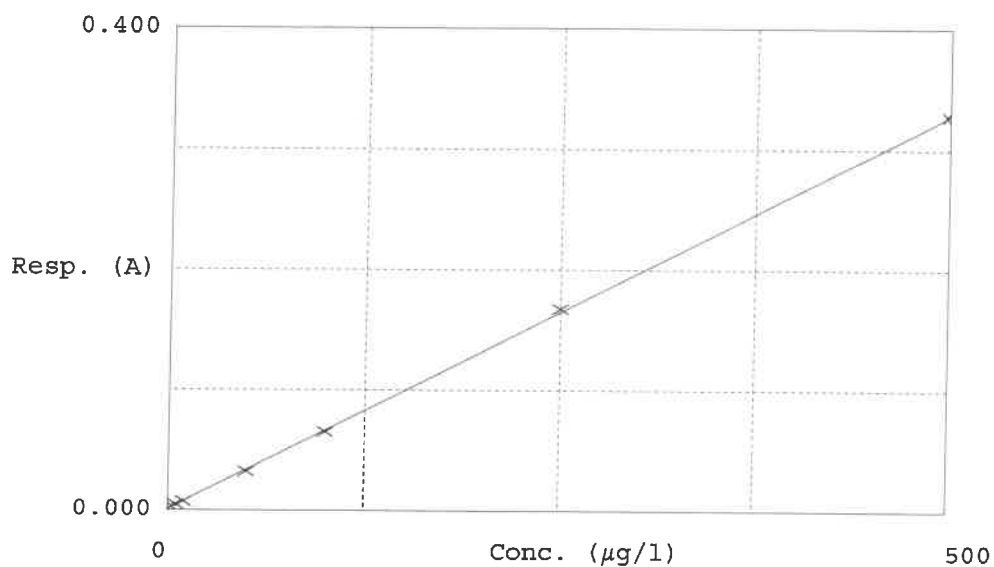

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	1.2464	0.0000	-
2	5.0PPBCN	0.005	5.7593	5.0000	15.2
3	10PPBCN	0.007	9.4359	10.0000	-5.6
4	50PPBCN	0.032	47.8745	50.0000	-4.3
5	100PPBCN	0.065	97.9471	100.0000	-2.1
6	250PPBCN	0.168	254.2198	250.0000	1.7
7	500PPBCN	0.327	498.5169	500.0000	-0.3

05/22/2024
RM