

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio n HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-051324	5/13/2024 15:40		IZ/MA
STD2	0.4450	0.6690	0.6700	2.1990	0.5620	1.1310	3.4510	IC1-051324	5/13/2024 16:02		IZ/MA
STD3	0.8040	1.2260	1.2290	4.0910	1.0210	1.9980	6.1260	IC1-051324	5/13/2024 16:23		IZ/MA
STD4	1.0000	1.4810	1.4990	4.9540	1.2400	2.5220	7.4370	IC1-051324	5/13/2024 16:45		IZ/MA
STD5	1.9530	2.9200	2.8930	9.7290	2.4170	4.8420	14.4330	IC1-051324	5/13/2024 17:06		IZ/MA
STD6	3.9170	5.8890	5.8830	19.6980	4.9170	9.7880	29.2960	IC1-051324	5/13/2024 17:27		IZ/MA
STD7	5.0810	7.6150	7.6260	25.3280	6.3430	12.7180	37.7560	IC1-051324	5/13/2024 17:49		IZ/MA

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	11.2500	11.5000	11.6667	9.9500	12.4000	13.1000	15.0333
STD3	0.5000	2.1667	2.4167	2.2750	2.1000	-0.1000	2.1000
STD4	0.0000	-1.2667	-0.0667	-0.9200	-0.8000	0.8800	-0.8400
STD5	-2.3500	-2.6667	-3.5667	-2.7100	-3.3200	-3.1600	-3.7800
STD6	-2.0750	-1.8500	-1.9500	-1.5100	-1.6600	-2.1200	-2.3467
STD7	1.6200	1.5333	1.6800	1.3120	1.4880	1.7440	2.0432

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

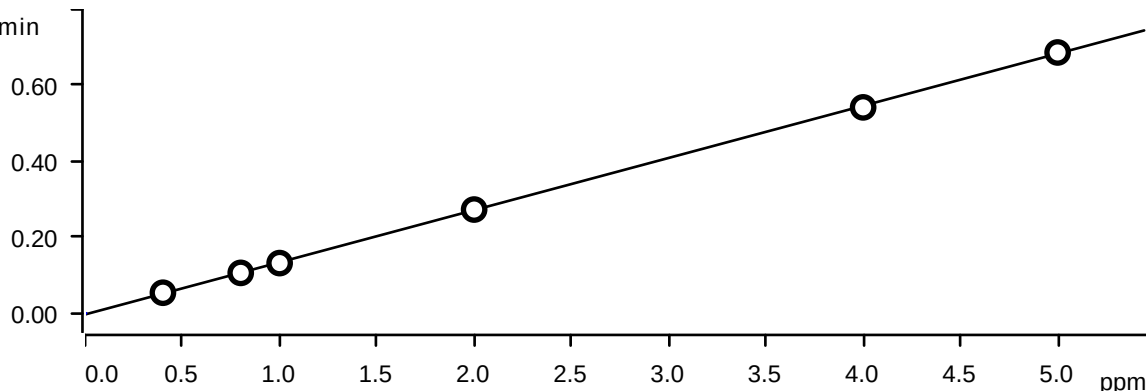

Function: $A = -3.05003E-3 + 0.0137350 \times Q$


Relative standard deviation 1.034950 %

Correlation coefficient 0.999943

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.054	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.106	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.132	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.273	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.542	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.687	Std 7	2024-04-13 01:04:41 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

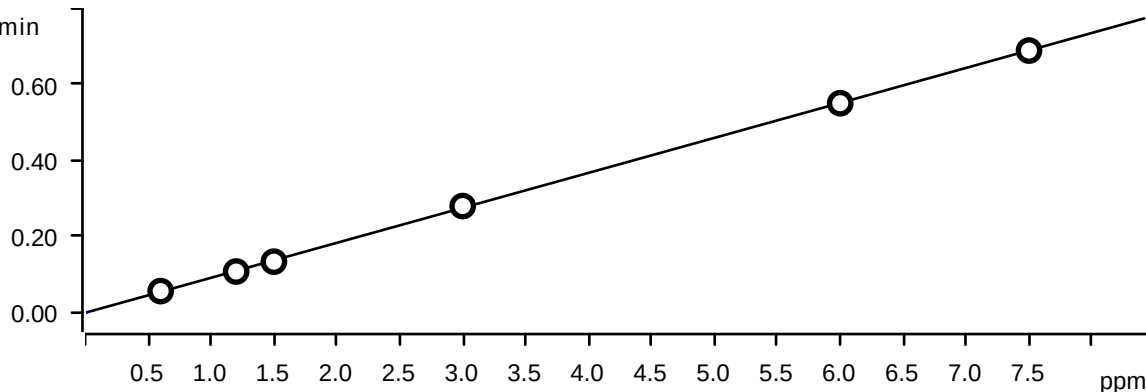

Function: $A = -1.03082E-3 + 9.21146E-3 \times Q$


Relative standard deviation 1.071537 %

Correlation coefficient 0.999938

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.056	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.108	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.134	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.280	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.551	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.689	Std 7	2024-04-13 01:04:41 UTC-4	used

Nitrite (Anions)


(μS/cm) x min

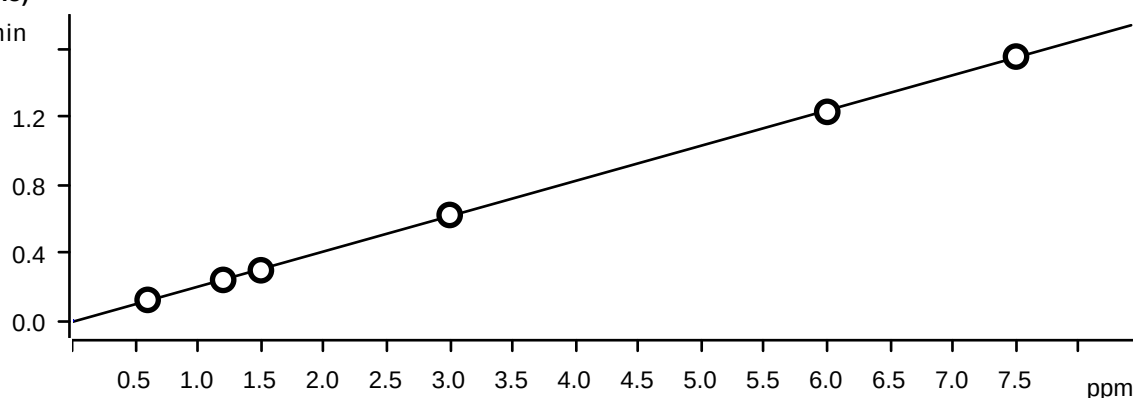Function: $A = -8.19751E-3 + 0.0207534 \times Q$

Relative standard deviation 1.139145 %

Correlation coefficient 0.999931


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.239	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.296	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.621	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.228	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.554	Std 7	2024-04-13 01:04:41 UTC-4	used

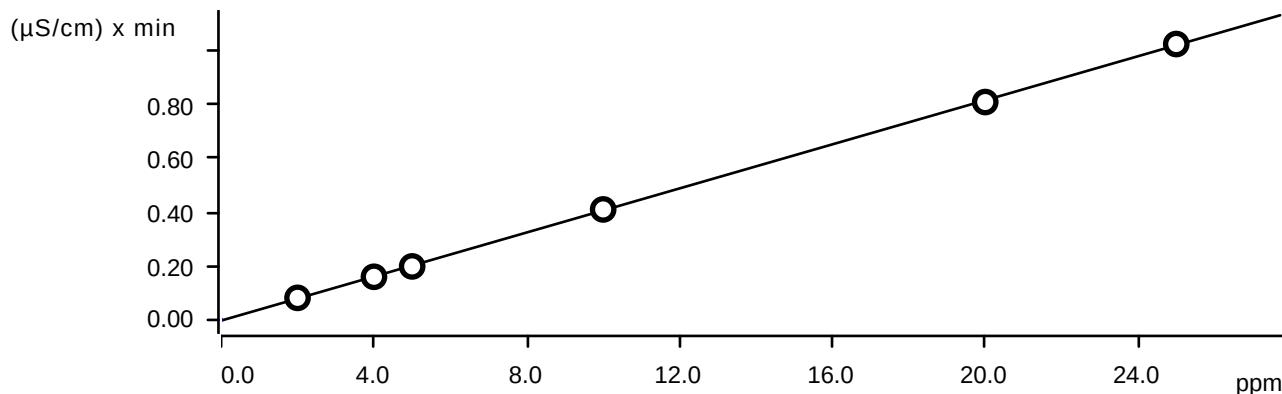Bromide (Anions)Function: $A = -2.93159E-3 + 4.09511E-3 \times Q$

Relative standard deviation 1.087762 %

Correlation coefficient 0.999936


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.082	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.160	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.199	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.410	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.810	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.025	Std 7	2024-04-13 01:04:41 UTC-4	used

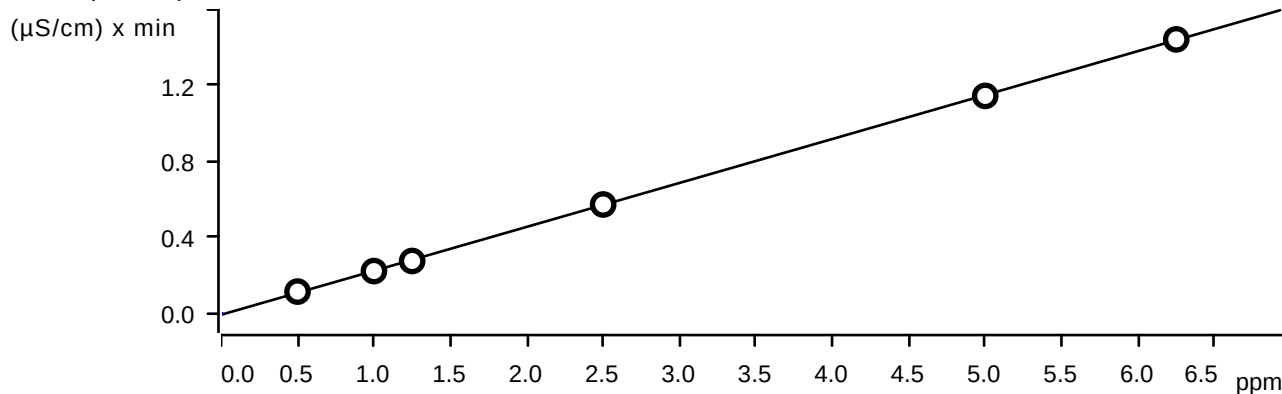Nitrate (Anions)Function: $A = -7.15004E-3 + 0.0231424 \times Q$

Relative standard deviation 0.870938 %

Correlation coefficient 0.999960

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.223	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.276	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.573	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.145	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.443	Std 7	2024-04-13 01:04:41 UTC-4	used

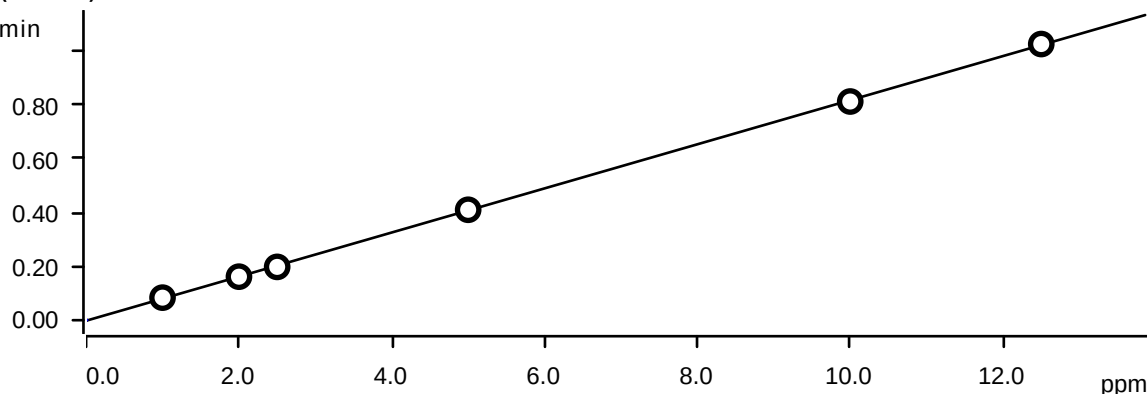
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -2.37452E-3 + 8.19864E-3 \times Q$

Relative standard deviation 1.011855 %

Correlation coefficient 0.999945

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.083	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.161	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.198	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.410	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.813	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.026	Std 7	2024-04-13 01:04:41 UTC-4	used

Sulfate (Anions)

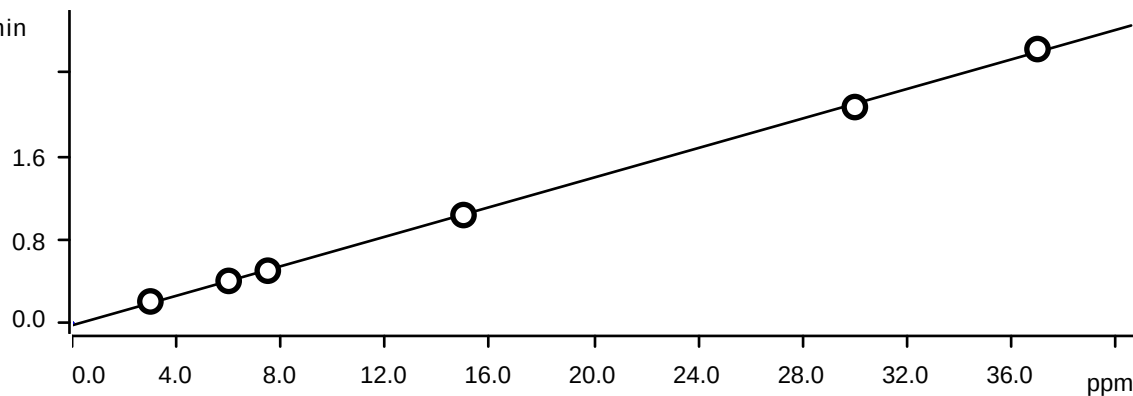 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0233221 + 7.09240E-3 \times Q$

Relative standard deviation 2.047074 %

Correlation coefficient 0.999778

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.206	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.403	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.501	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.035	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.072	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.629	Std 7	2024-04-13 01:04:41 UTC-4	used


Sample data

Ident Std 1
Sample type Standard 1
Determination start 2024-04-12 22:45:19 UTC-4
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

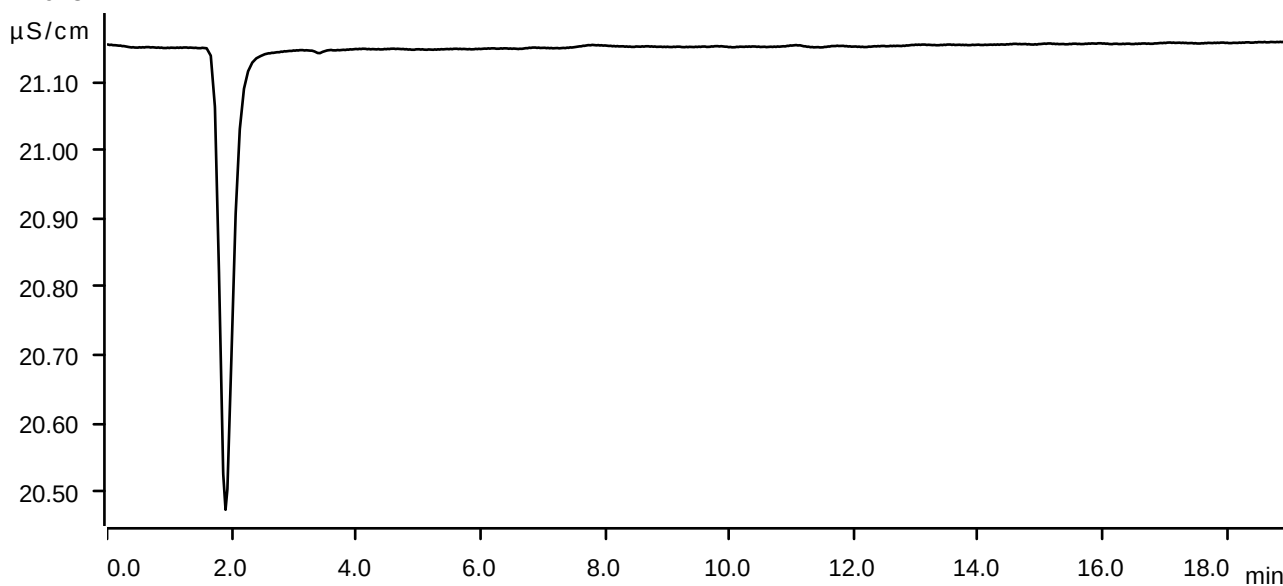


Sample data

Ident Std 2
Sample type Standard 2
Determination start 2024-04-12 23:06:41 UTC-4
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

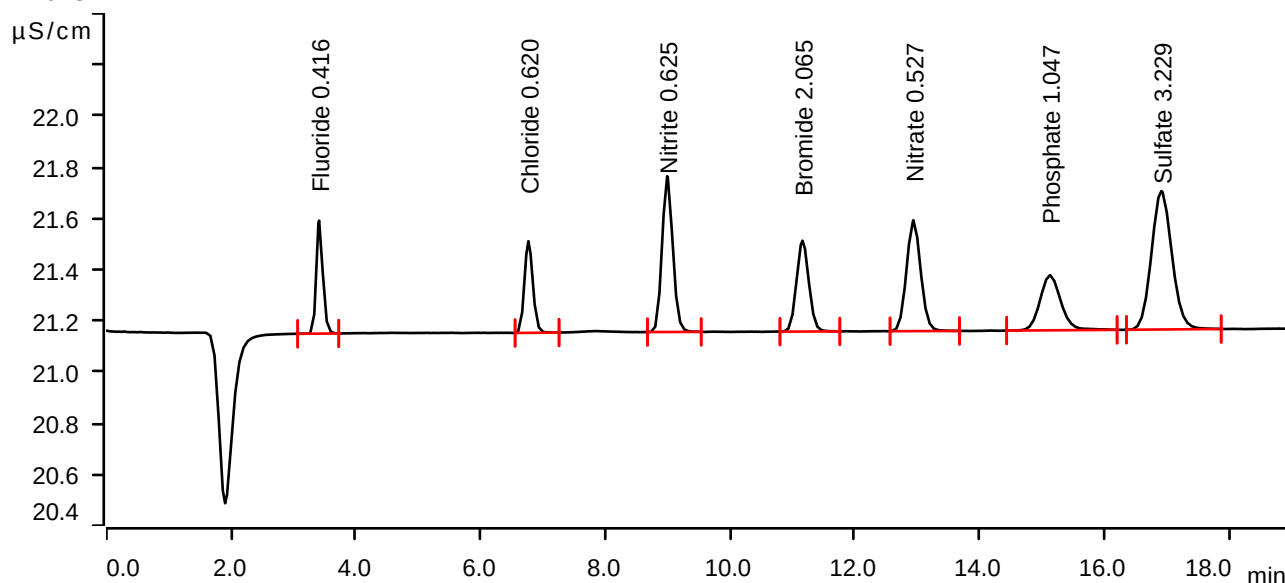

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.412	0.0541	0.441	0.416	Fluoride
2	6.767	0.0561	0.358	0.620	Chloride
3	8.993	0.1216	0.608	0.625	Nitrite
4	11.162	0.0816	0.355	2.065	Bromide
5	12.940	0.1148	0.433	0.527	Nitrate
6	15.127	0.0834	0.215	1.047	Phosphate
7	16.915	0.2057	0.541	3.229	Sulfate


Sample data

Ident Std 3
Sample type Standard 3
Determination start 2024-04-12 22:38:39 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.5 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

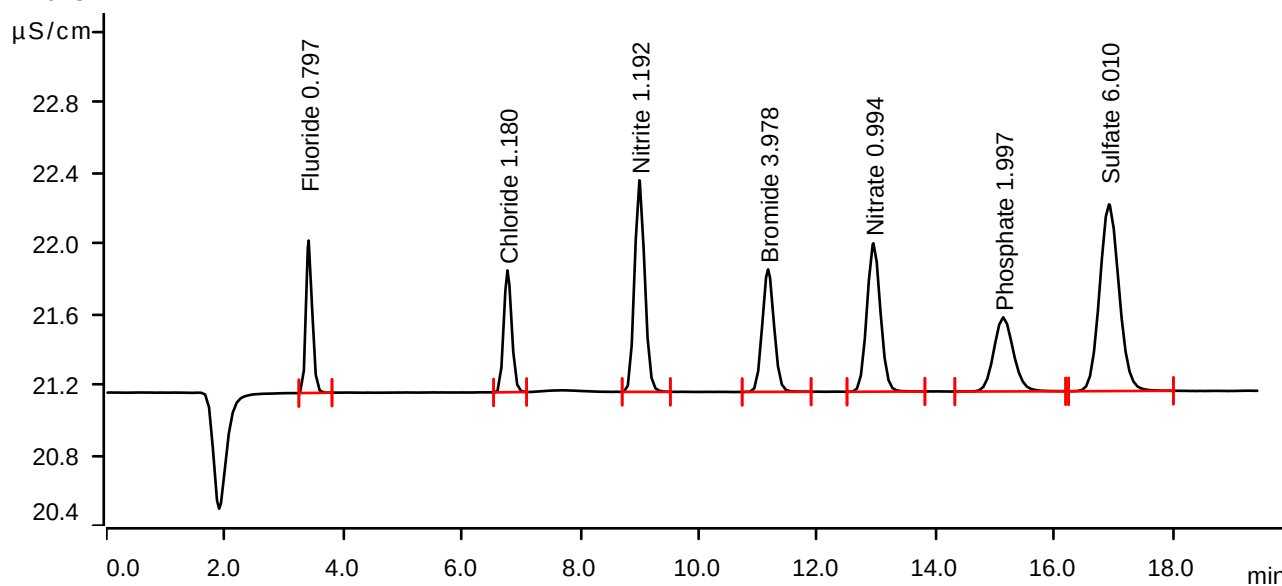

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.1064	0.863	0.797	Fluoride
2	6.770	0.1076	0.690	1.180	Chloride
3	8.997	0.2391	1.198	1.192	Nitrite
4	11.167	0.1600	0.694	3.978	Bromide
5	12.945	0.2229	0.840	0.994	Nitrate
6	15.137	0.1614	0.420	1.997	Phosphate
7	16.922	0.4029	1.057	6.010	Sulfate


Sample data

Ident Std 4
Sample type Standard 4
Determination start 2024-04-12 23:00:33 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

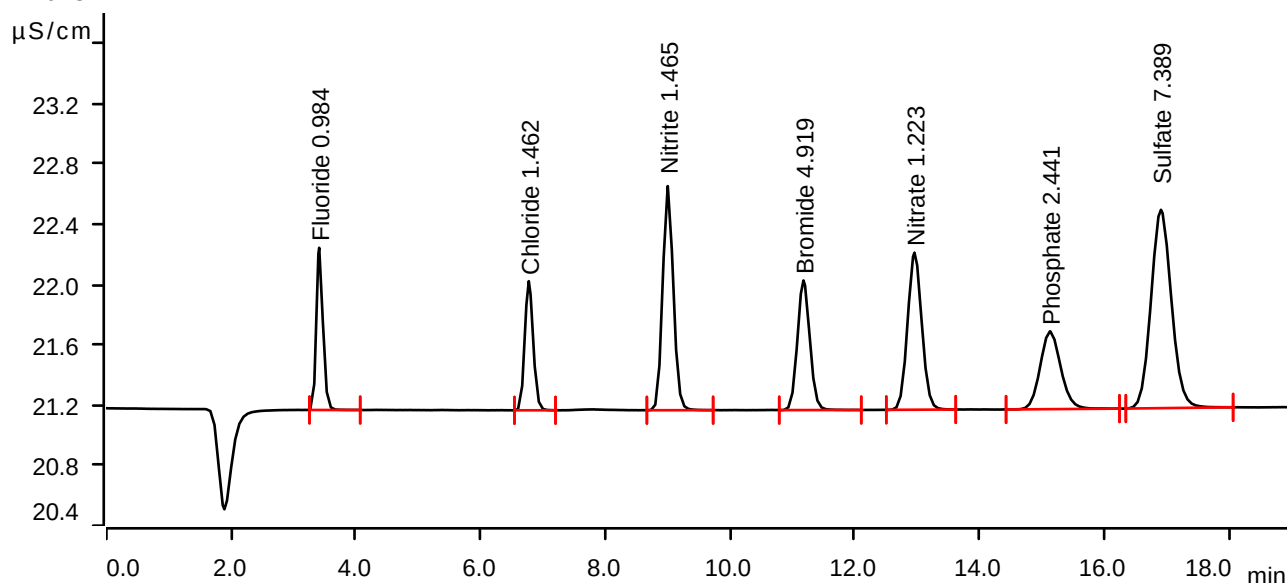

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.1321	1.077	0.984	Fluoride
2	6.773	0.1336	0.857	1.462	Chloride
3	9.002	0.2959	1.487	1.465	Nitrite
4	11.177	0.1985	0.861	4.919	Bromide
5	12.957	0.2759	1.043	1.223	Nitrate
6	15.128	0.1978	0.517	2.441	Phosphate
7	16.908	0.5007	1.317	7.389	Sulfate


Sample data

Ident Std 5
Sample type Standard 5
Determination start 2024-04-12 23:21:58 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

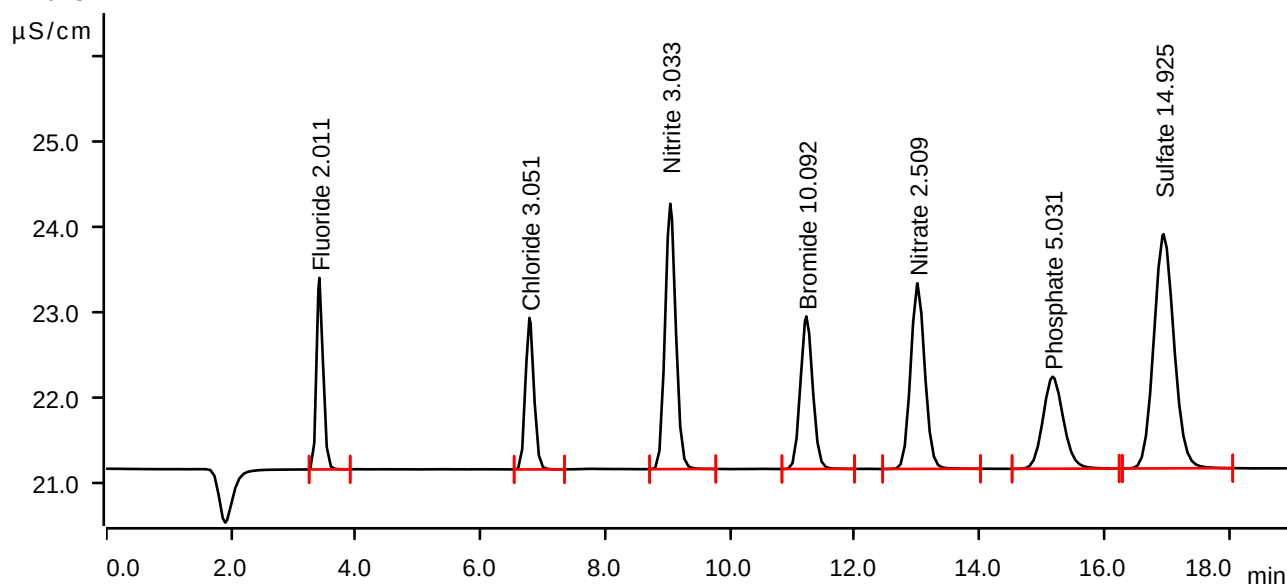

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.417	0.2731	2.244	2.011	Fluoride
2	6.783	0.2800	1.776	3.051	Chloride
3	9.042	0.6213	3.109	3.033	Nitrite
4	11.223	0.4104	1.788	10.092	Bromide
5	13.005	0.5735	2.175	2.509	Nitrate
6	15.172	0.4101	1.078	5.031	Phosphate
7	16.950	1.0352	2.744	14.925	Sulfate


Sample data

Ident Std 6
Sample type Standard 6
Determination start 2024-04-12 23:43:14 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

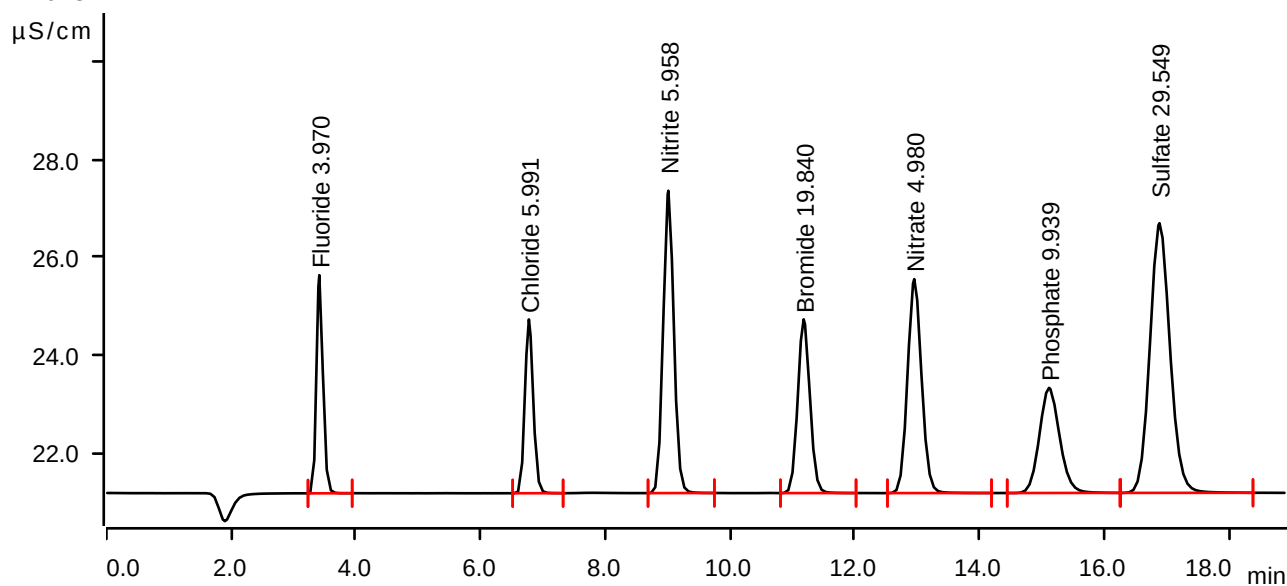

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.5422	4.473	3.970	Fluoride
2	6.775	0.5509	3.563	5.991	Chloride
3	9.012	1.2283	6.198	5.958	Nitrite
4	11.180	0.8095	3.562	19.840	Bromide
5	12.953	1.1453	4.386	4.980	Nitrate
6	15.113	0.8125	2.155	9.939	Phosphate
7	16.885	2.0724	5.528	29.549	Sulfate


Sample data

Ident Std 7
Sample type Standard 7
Determination start 2024-04-13 00:04:41 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

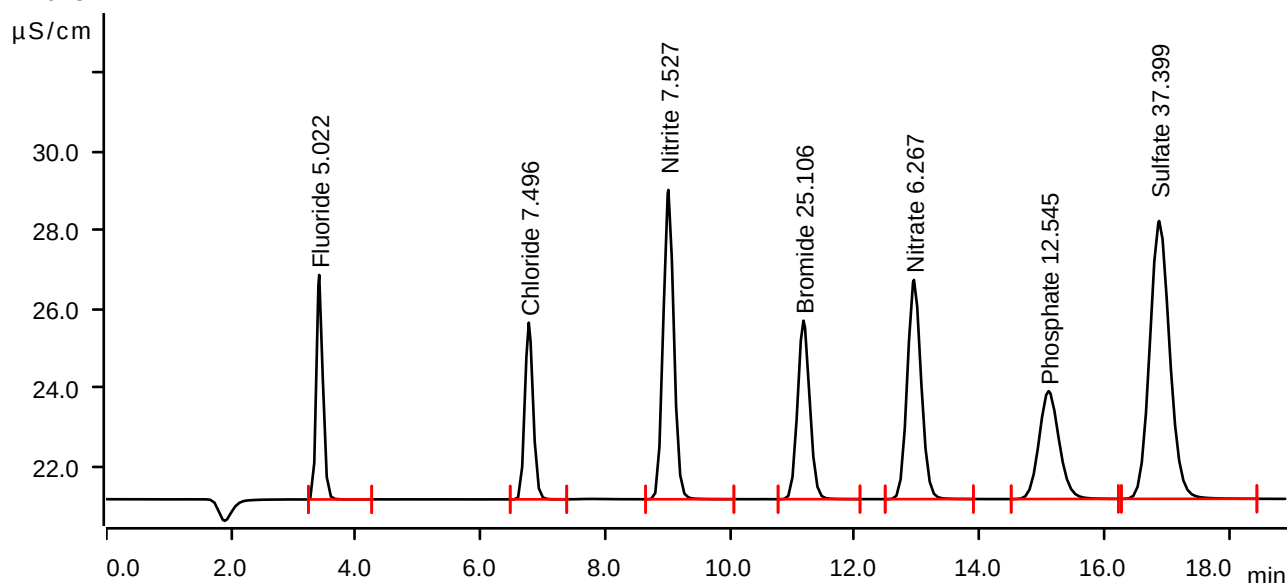

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.6867	5.697	5.022	Fluoride
2	6.773	0.6894	4.484	7.496	Chloride
3	9.012	1.5538	7.851	7.527	Nitrite
4	11.177	1.0252	4.531	25.106	Bromide
5	12.948	1.4431	5.565	6.267	Nitrate
6	15.107	1.0261	2.739	12.545	Phosphate
7	16.880	2.6292	7.053	37.399	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-04-13 02:35:03 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

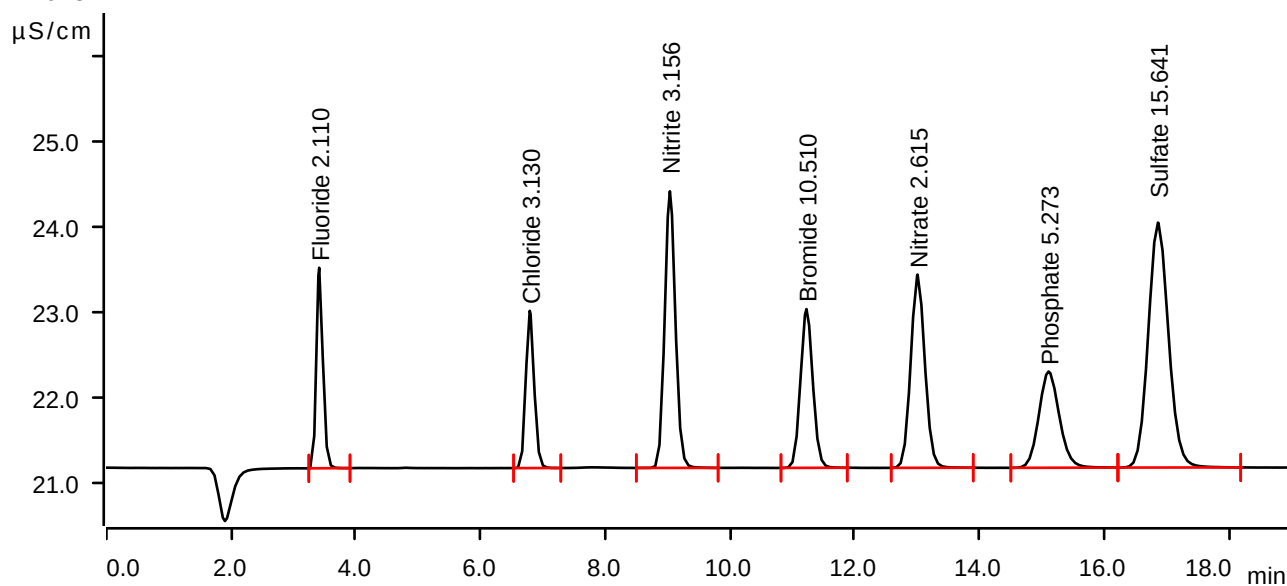


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.2867	2.349	2.110	Fluoride
2	6.788	0.2873	1.842	3.130	Chloride
3	9.035	0.6468	3.241	3.156	Nitrite
4	11.225	0.4275	1.860	10.510	Bromide
5	13.007	0.5980	2.263	2.615	Nitrate
6	15.107	0.4300	1.127	5.273	Phosphate
7	16.860	1.0860	2.869	15.641	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2024-04-13 02:56:34 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

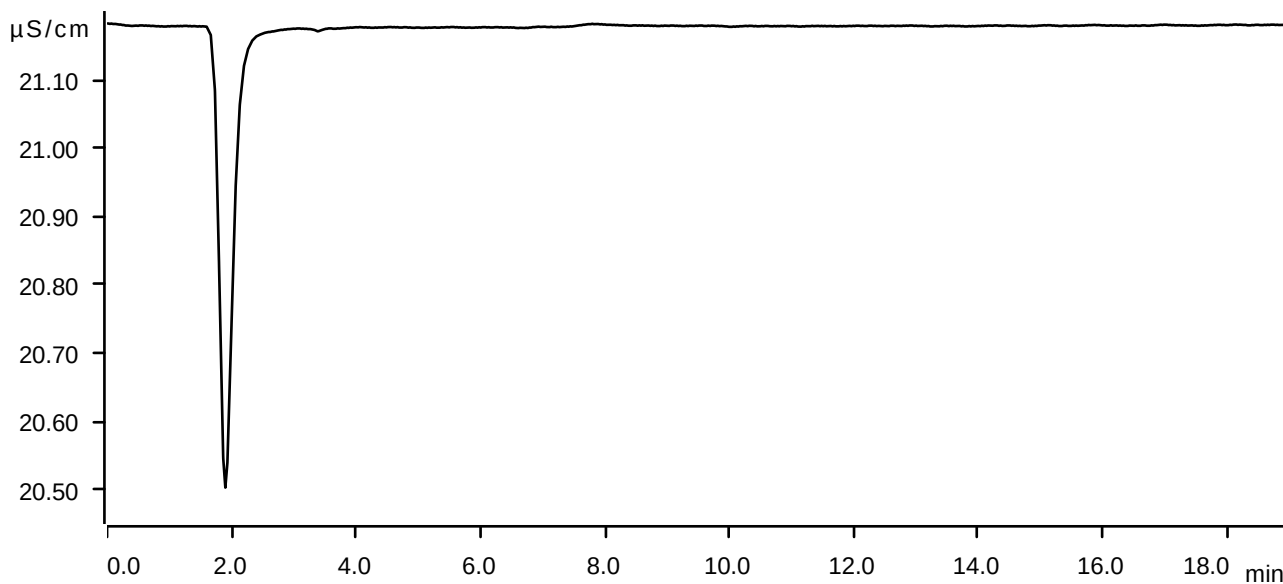Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-05 18:27:33 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

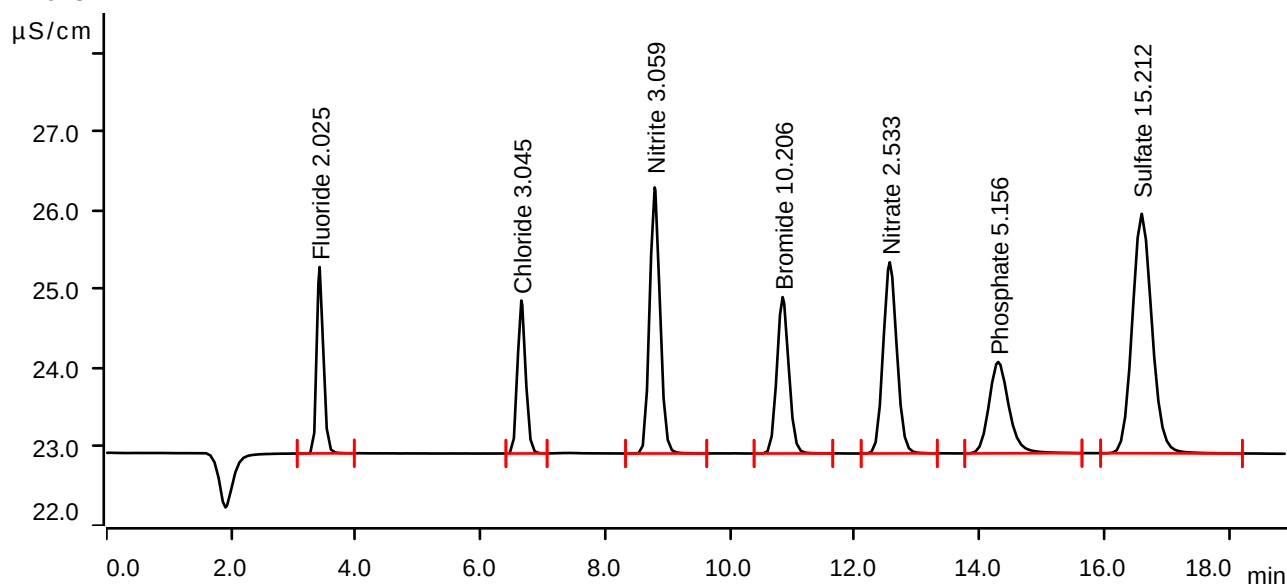

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.420	0.2891	2.366	2.025	Fluoride
2	6.653	0.2946	1.941	3.045	Chloride
3	8.792	0.6523	3.376	3.059	Nitrite
4	10.843	0.4390	1.985	10.206	Bromide
5	12.560	0.6140	2.426	2.533	Nitrate
6	14.298	0.4293	1.160	5.156	Phosphate
7	16.598	1.1151	3.039	15.212	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-05 18:49:03 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

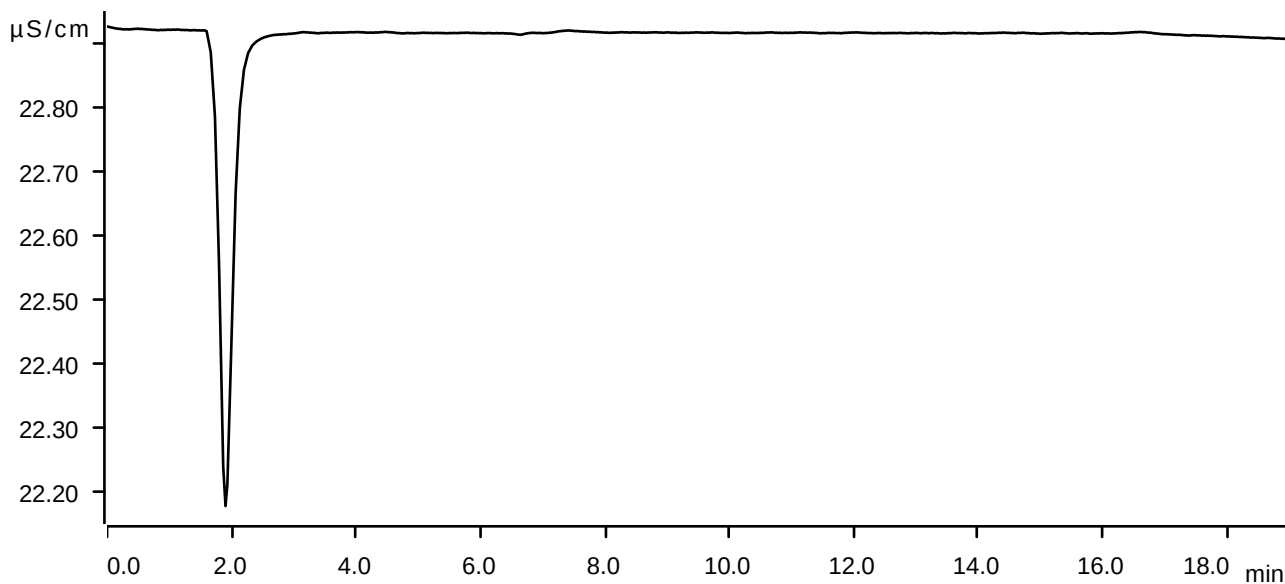


Sample data

Ident LB131125BLW
Sample type Sample
Determination start 2024-06-05 19:10:32 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

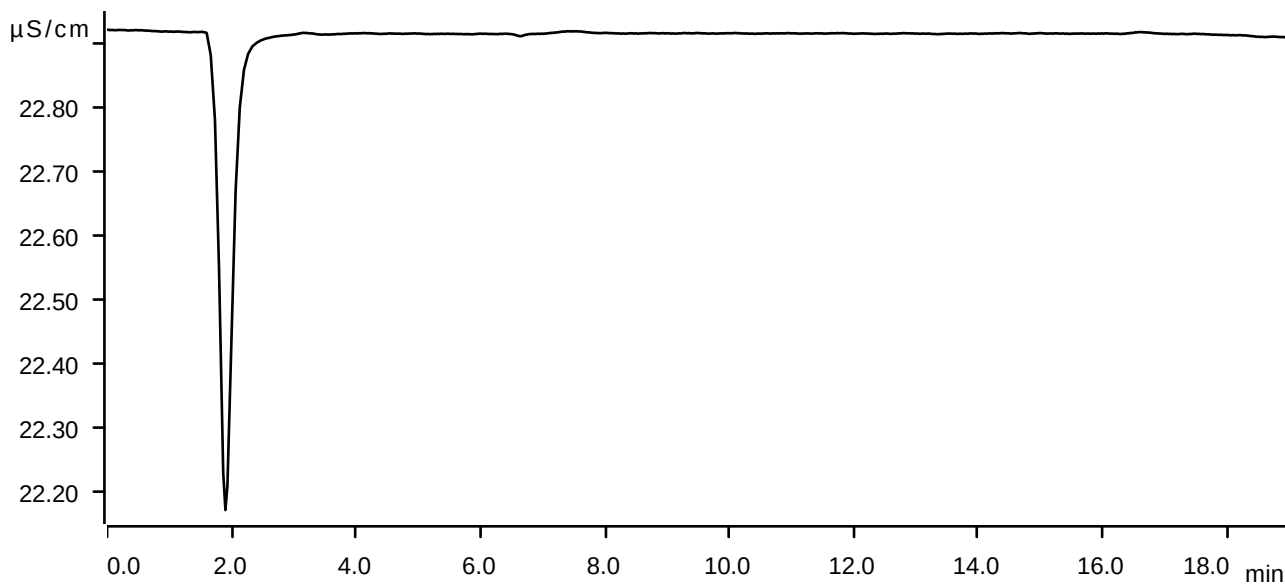


Sample data

Ident LB131125BSW
Sample type Check standard 1
Determination start 2024-06-05 19:32:03 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

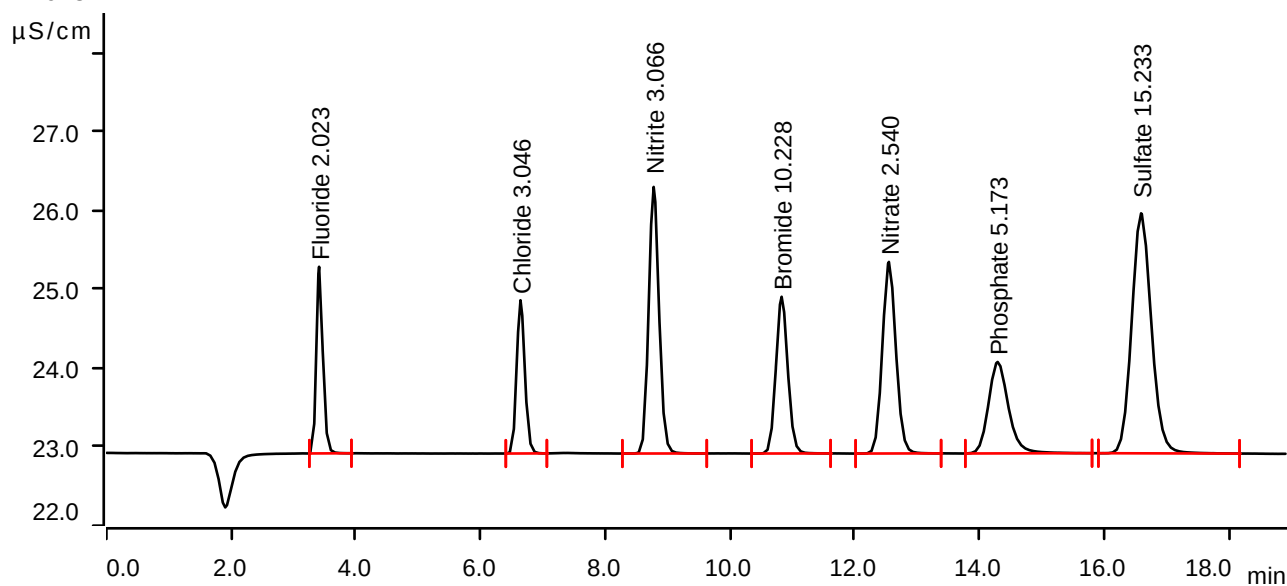

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.412	0.2888	2.369	2.023	Fluoride
2	6.640	0.2947	1.945	3.046	Chloride
3	8.775	0.6539	3.383	3.066	Nitrite
4	10.827	0.4400	1.989	10.228	Bromide
5	12.547	0.6158	2.431	2.540	Nitrate
6	14.290	0.4307	1.161	5.173	Phosphate
7	16.590	1.1167	3.046	15.233	Sulfate


Sample data

Ident P2749-01
Sample type Sample
Determination start 2024-06-05 19:53:36 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

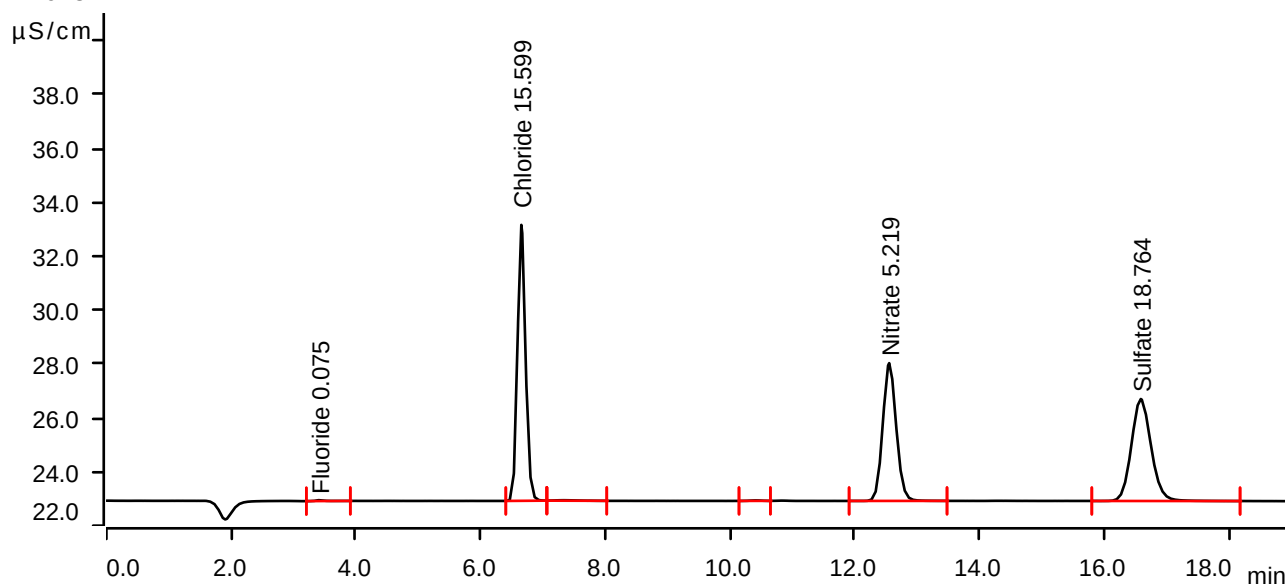

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.410	0.0053	0.033	0.075	Fluoride
2	6.653	1.5295	10.236	15.599	Chloride
3	7.337	0.0074	0.018	invalid	
4	10.417	0.0035	0.017	invalid	
5	12.552	1.2797	5.111	5.219	Nitrate
6	16.585	1.3848	3.783	18.764	Sulfate


Sample data

Ident P2749-01MS
Sample type Sample
Determination start 2024-06-05 20:15:04 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

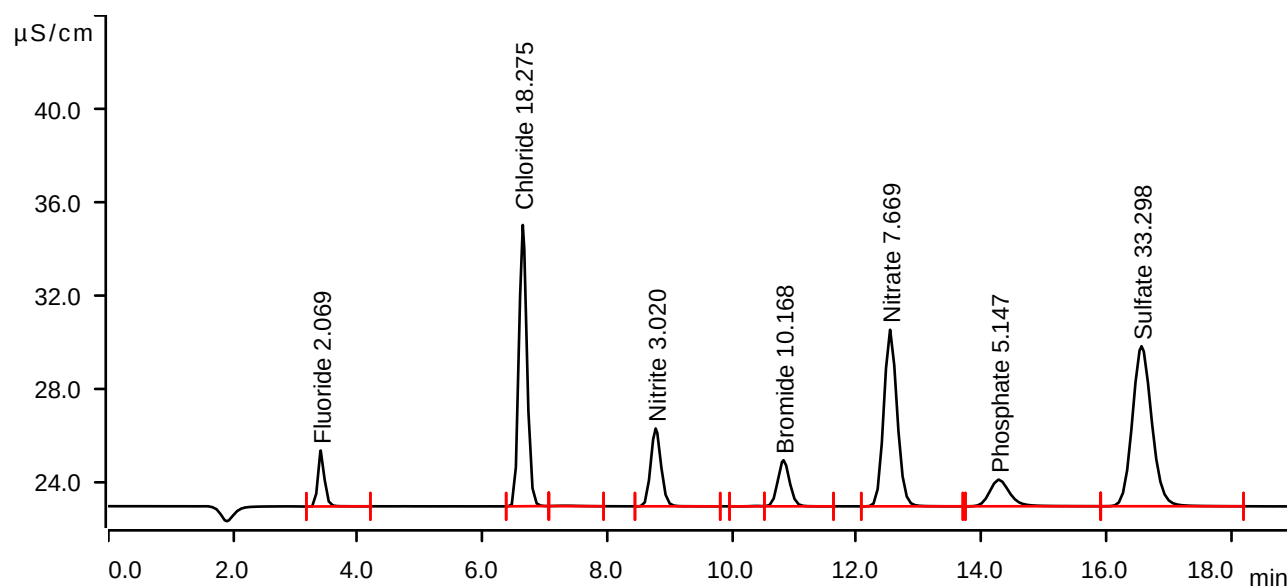

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.405	0.2956	2.403	2.069	Fluoride
2	6.645	1.7926	12.081	18.275	Chloride
3	7.307	0.0068	0.017	invalid	
4	8.775	0.6437	3.344	3.020	Nitrite
5	10.388	0.0035	0.017	invalid	
6	10.825	0.4374	1.980	10.168	Bromide
7	12.533	1.8871	7.583	7.669	Nitrate
8	14.277	0.4285	1.144	5.147	Phosphate
9	16.565	2.4883	6.872	33.298	Sulfate


Sample data

Ident P2749-01MSD
Sample type Sample
Determination start 2024-06-05 20:36:32 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

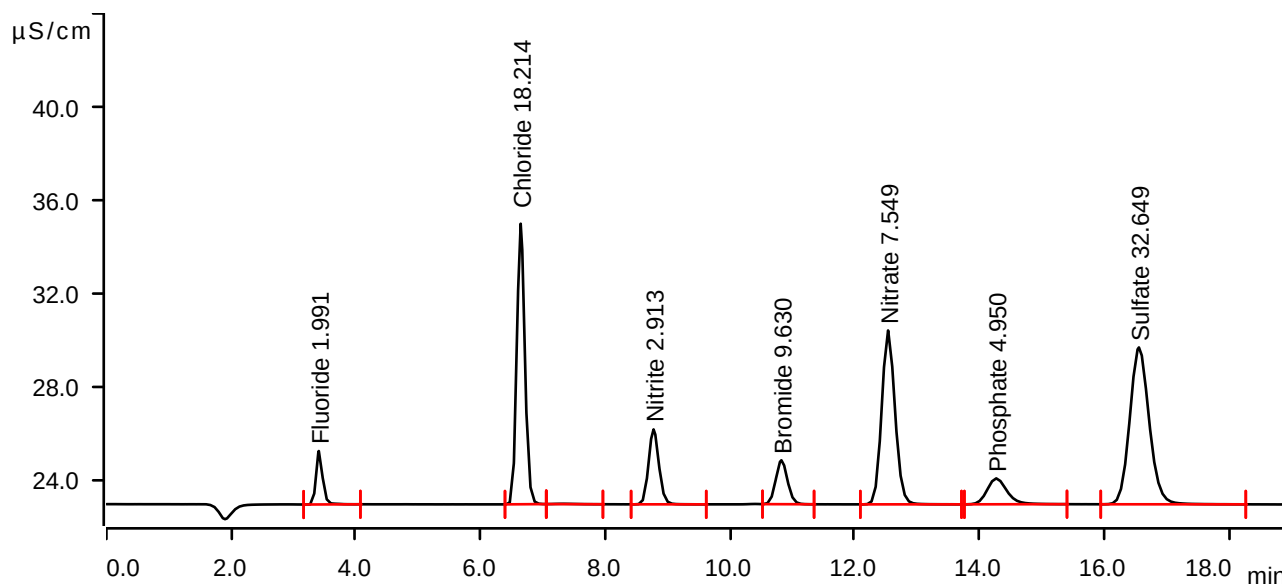

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.407	0.2842	2.295	1.991	Fluoride
2	6.643	1.7866	12.050	18.214	Chloride
3	7.323	0.0060	0.016	invalid	
4	8.773	0.6201	3.219	2.913	Nitrite
5	10.823	0.4137	1.887	9.630	Bromide
6	12.533	1.8571	7.469	7.549	Nitrate
7	14.268	0.4117	1.111	4.950	Phosphate
8	16.555	2.4390	6.736	32.649	Sulfate


Sample data

Ident P2749-03
Sample type Sample
Determination start 2024-06-05 21:19:20 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

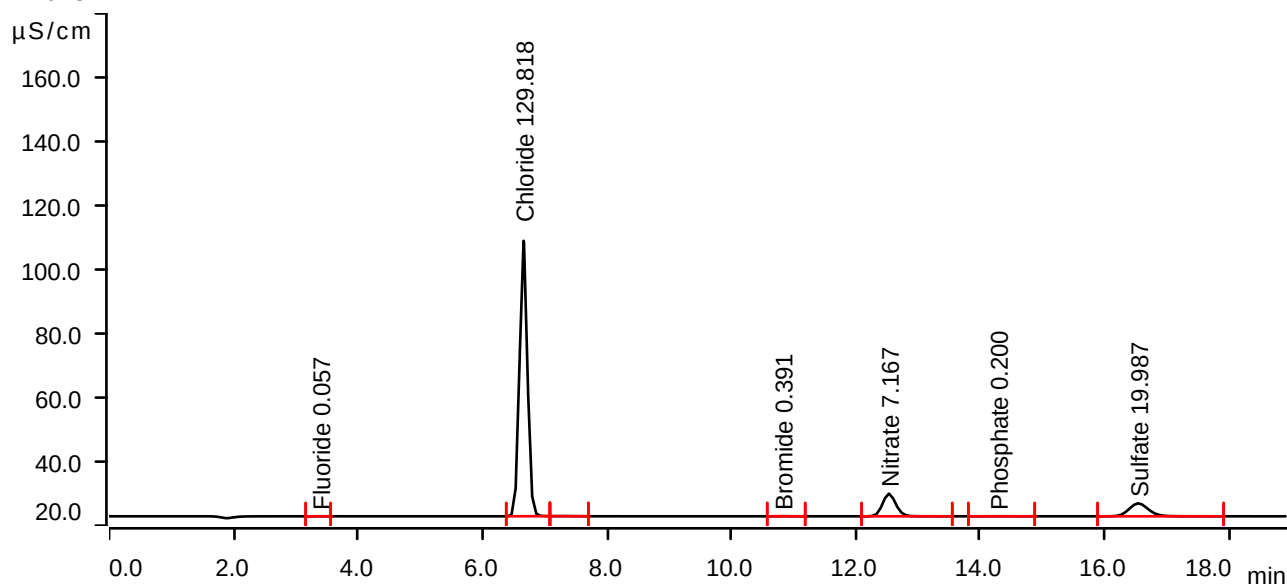

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.0026	0.020	0.057	Fluoride
2	6.662	12.7641	86.042	129.818	Chloride
3	7.262	0.0061	0.020	invalid	
4	10.817	0.0072	0.032	0.391	Bromide
5	12.532	1.7626	7.074	7.167	Nitrate
6	14.283	0.0059	0.015	0.200	Phosphate
7	16.538	1.4776	4.053	19.987	Sulfate


Sample data

Ident P2749-05
Sample type Sample
Determination start 2024-06-05 21:40:46 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

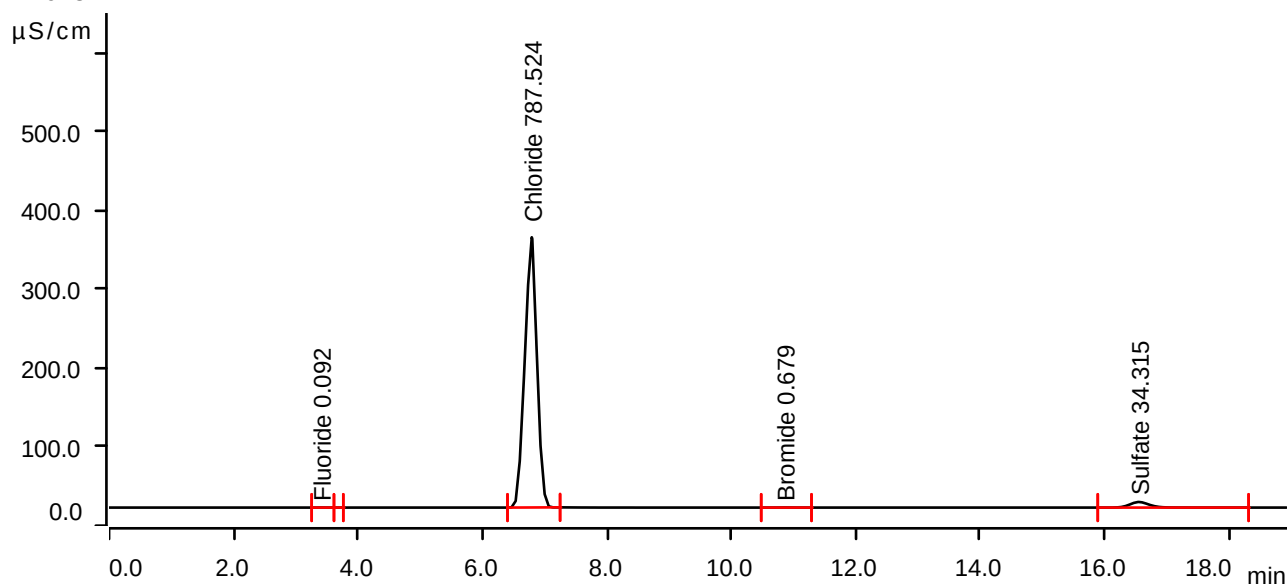

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.403	0.0078	0.062	0.092	Fluoride
2	3.633	0.0001	0.001	invalid	
3	6.793	77.4566	342.918	787.524	Chloride
4	10.857	0.0198	0.090	0.679	Bromide
5	16.548	2.5655	7.107	34.315	Sulfate


Sample data

Ident P2749-07
Sample type Sample
Determination start 2024-06-05 22:23:32 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

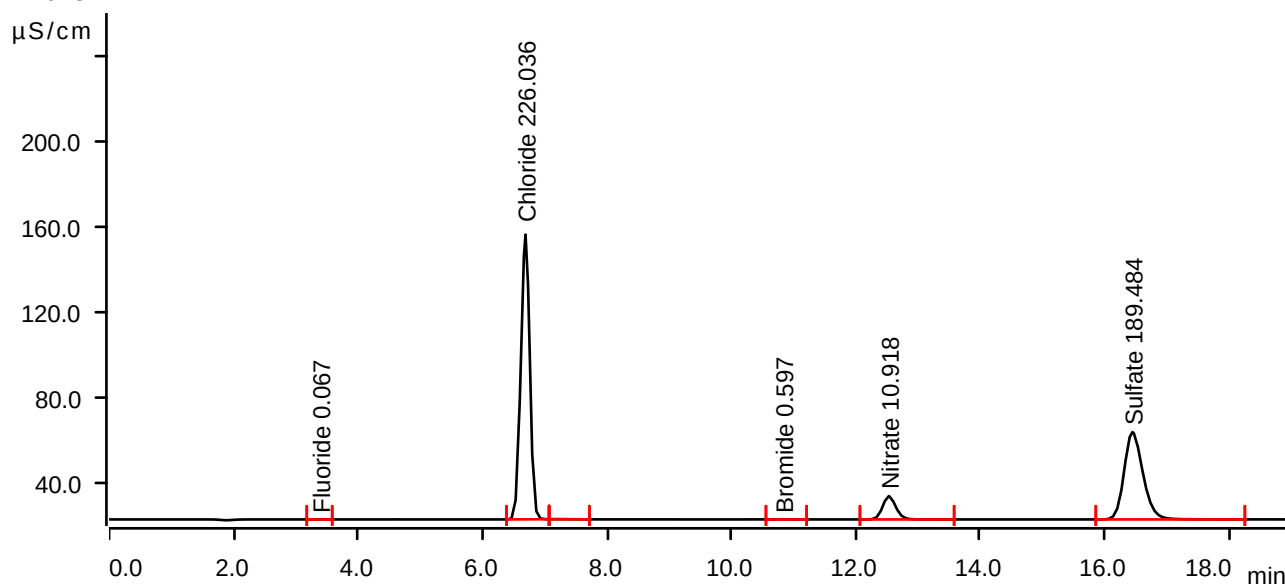

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.0041	0.033	0.067	Fluoride
2	6.693	22.2282	133.393	226.036	Chloride
3	7.232	0.0110	0.035	invalid	
4	10.828	0.0163	0.074	0.597	Bromide
5	12.532	2.6922	10.942	10.918	Nitrate
6	16.445	14.3466	40.920	189.484	Sulfate


Sample data

Ident P2749-09
Sample type Sample
Determination start 2024-06-05 23:06:18 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

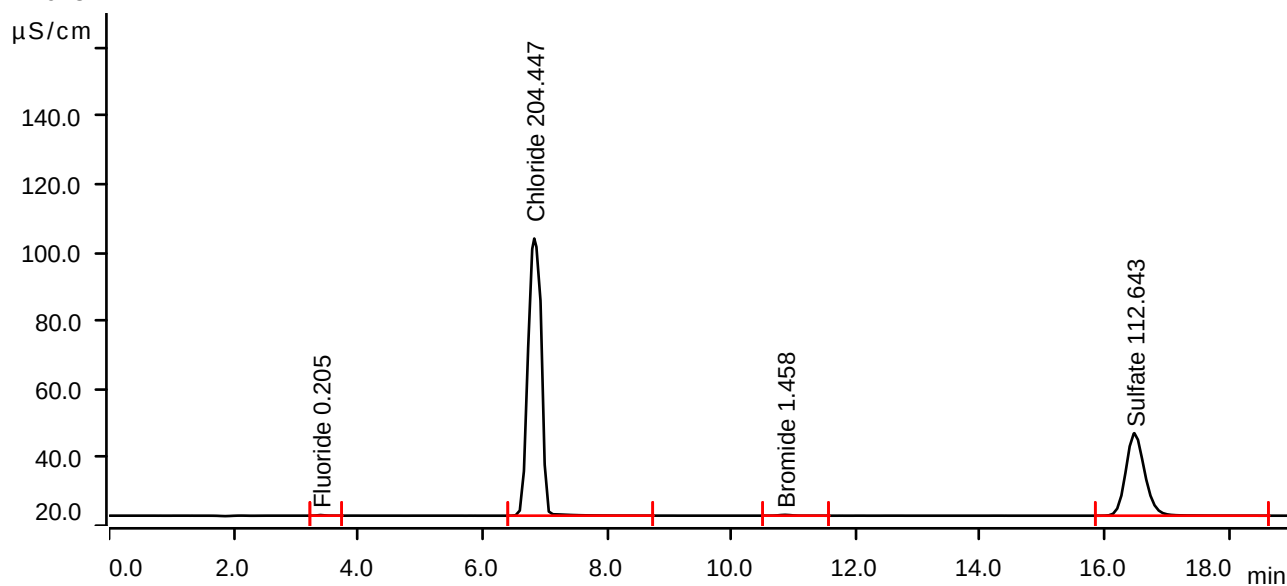

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.0242	0.191	0.205	Fluoride
2	6.833	20.1046	81.167	204.447	Chloride
3	10.862	0.0541	0.242	1.458	Bromide
4	16.477	8.5125	24.158	112.643	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-05 23:27:42 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

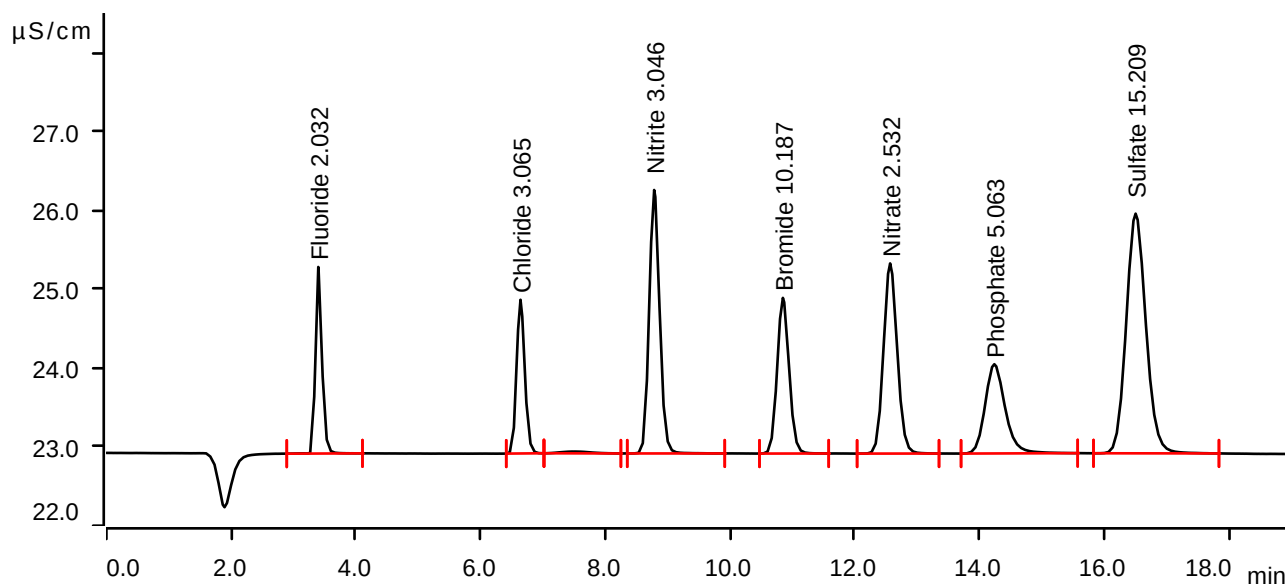

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.398	0.2902	2.367	2.032	Fluoride
2	6.640	0.2966	1.950	3.065	Chloride
3	7.512	0.0126	0.023	invalid	
4	8.783	0.6494	3.343	3.046	Nitrite
5	10.847	0.4382	1.975	10.187	Bromide
6	12.567	0.6138	2.413	2.532	Nitrate
7	14.237	0.4213	1.133	5.063	Phosphate
8	16.502	1.1149	3.042	15.209	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-05 23:49:12 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

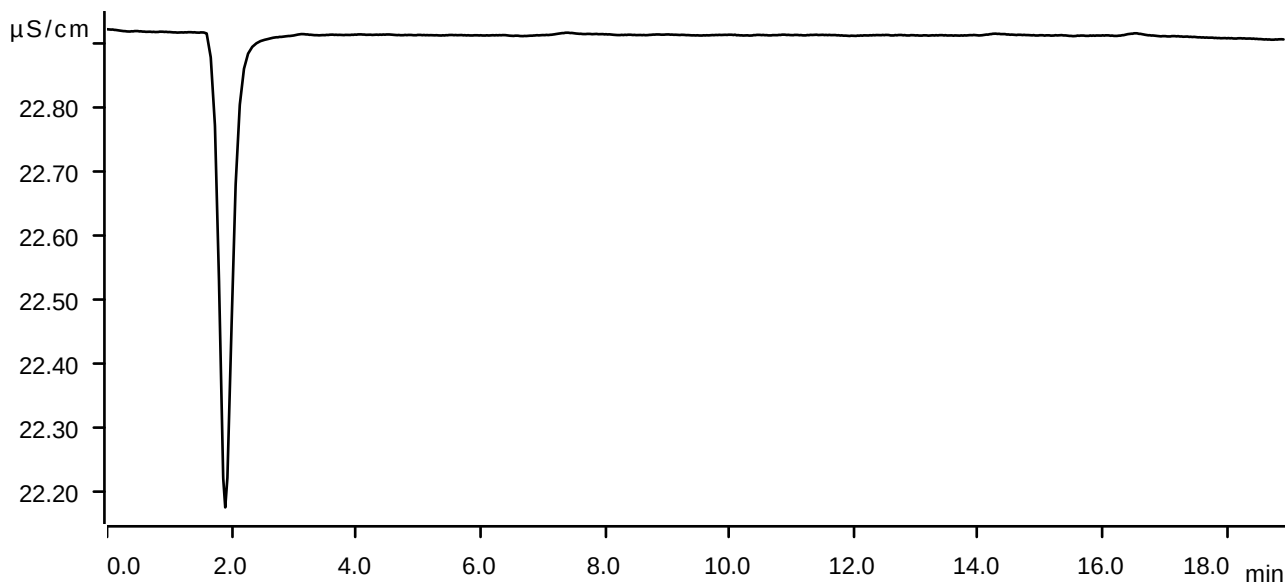


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-06 09:49:37 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

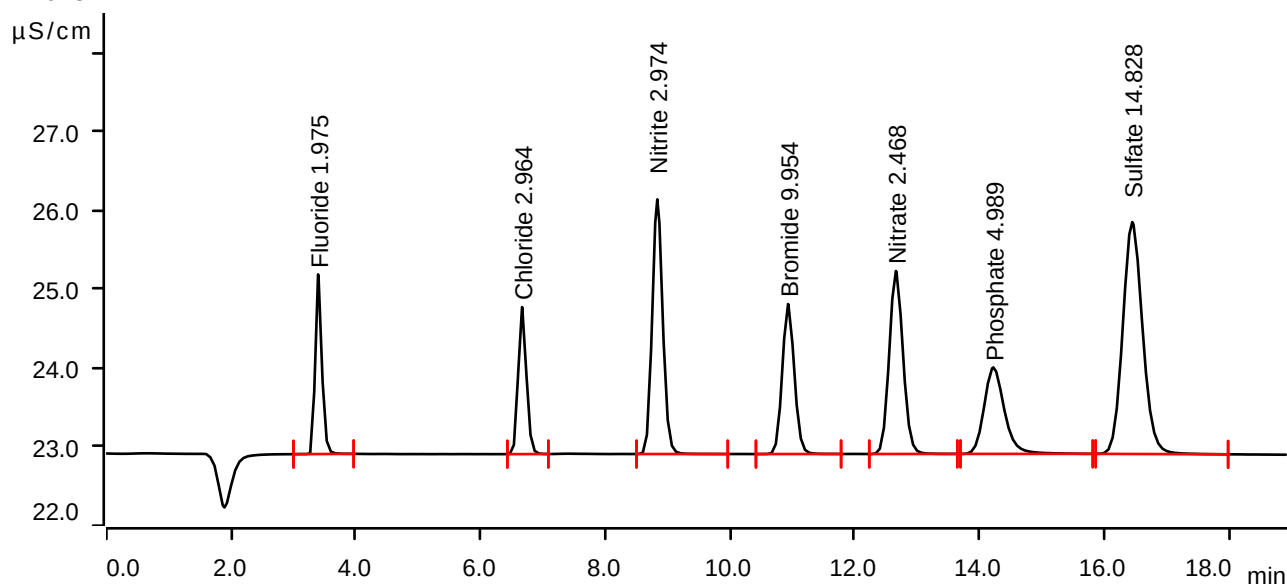

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.2819	2.280	1.975	Fluoride
2	6.665	0.2866	1.865	2.964	Chloride
3	8.833	0.6336	3.231	2.974	Nitrite
4	10.930	0.4280	1.903	9.954	Bromide
5	12.658	0.5980	2.322	2.468	Nitrate
6	14.222	0.4151	1.098	4.989	Phosphate
7	16.448	1.0859	2.943	14.828	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-06 10:11:07 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

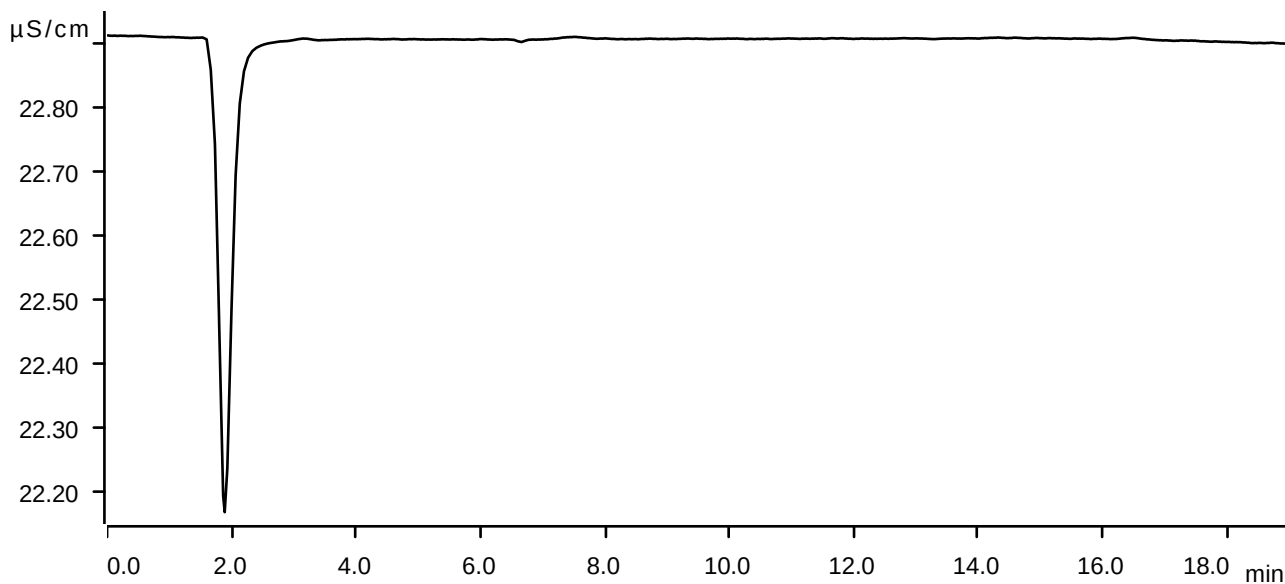


Sample data

Ident LB131125BLW2
Sample type Sample
Determination start 2024-06-06 10:32:37 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

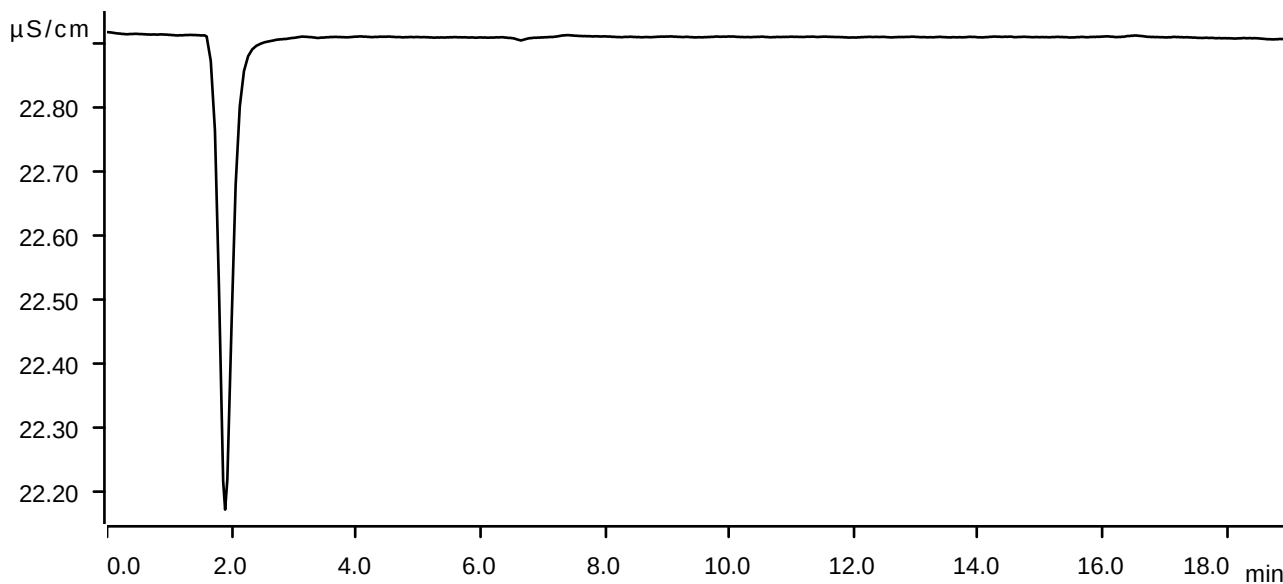


Sample data

Ident LB131125BSW2
Sample type Check standard 1
Determination start 2024-06-06 10:54:07 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

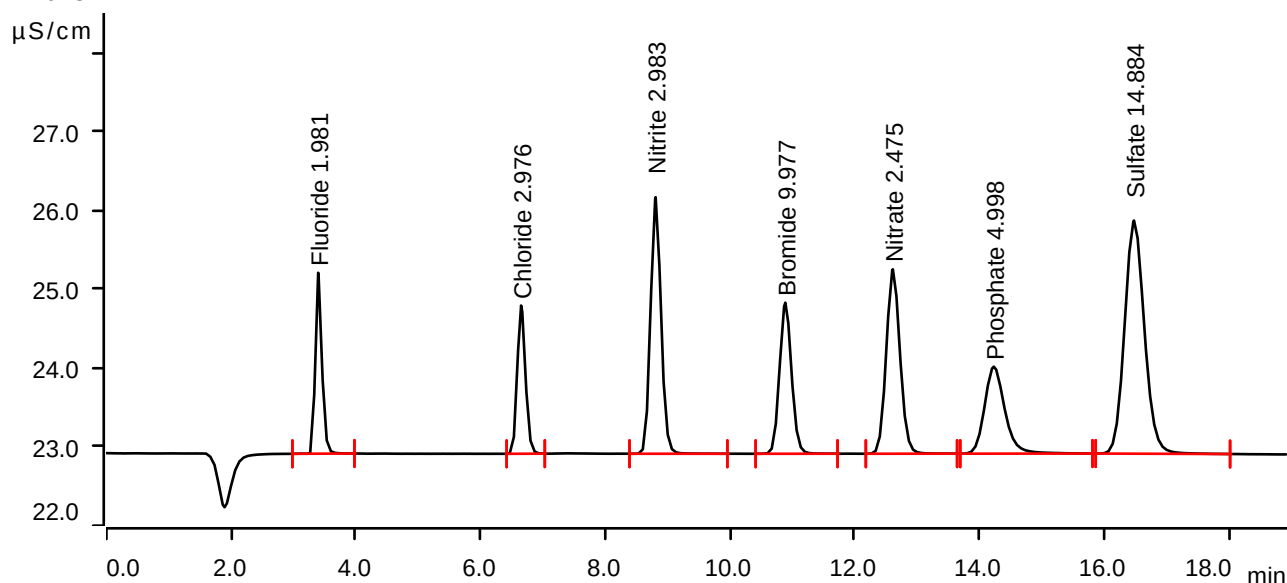

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.2828	2.296	1.981	Fluoride
2	6.650	0.2879	1.881	2.976	Chloride
3	8.807	0.6356	3.256	2.983	Nitrite
4	10.887	0.4290	1.917	9.977	Bromide
5	12.610	0.5997	2.340	2.475	Nitrate
6	14.228	0.4158	1.104	4.998	Phosphate
7	16.477	1.0902	2.959	14.884	Sulfate


Sample data

Ident P2749-01DLX5
Sample type Sample
Determination start 2024-06-06 11:15:39 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

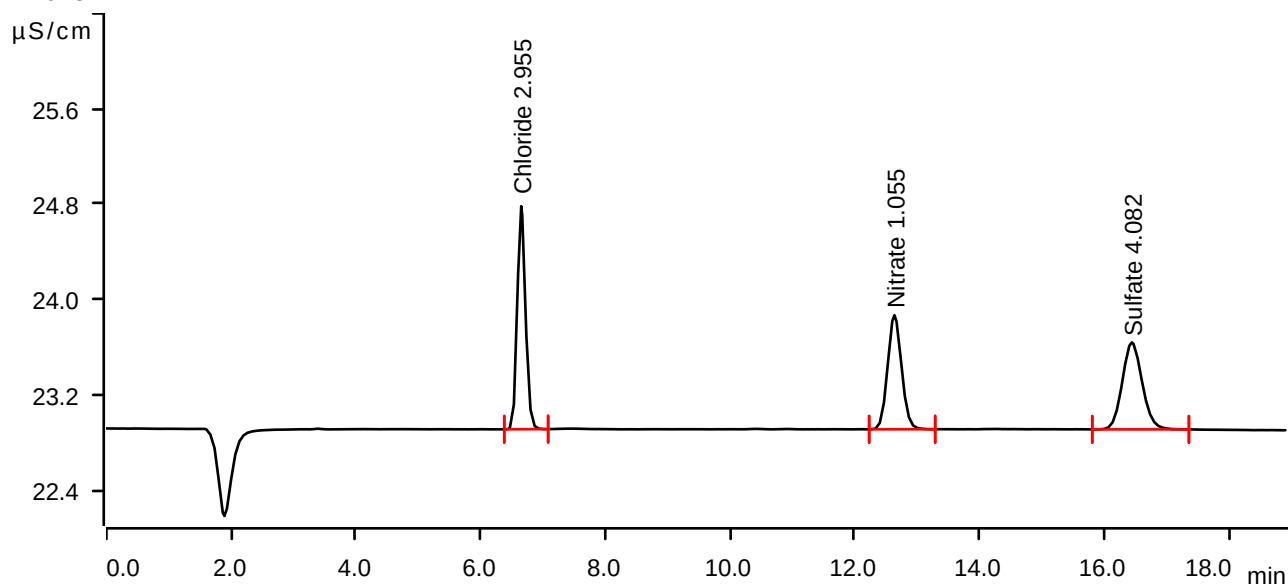

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.652	0.2858	1.872	2.955	Chloride
2	12.635	0.2477	0.958	1.055	Nitrate
3	16.442	0.2700	0.731	4.082	Sulfate


Sample data

Ident P2749-03DLX50
Sample type Sample
Determination start 2024-06-06 11:37:12 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

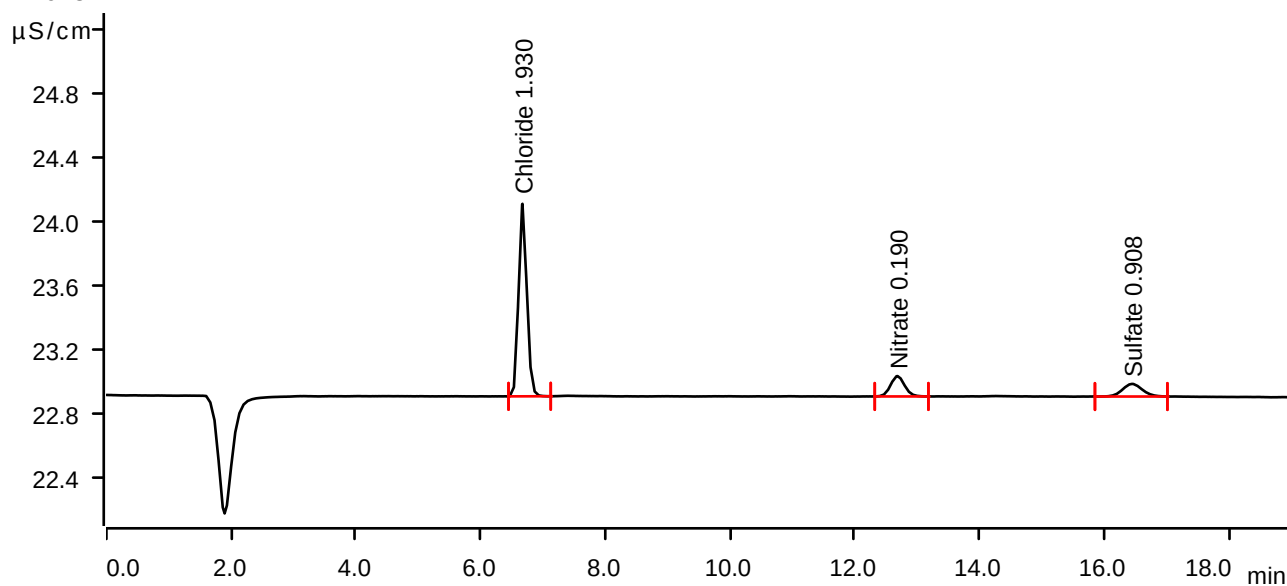

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.672	0.1850	1.203	1.930	Chloride
2	12.685	0.0332	0.127	0.190	Nitrate
3	16.443	0.0291	0.079	0.908	Sulfate


Sample data

Ident P2749-05DLX200
Sample type Sample
Determination start 2024-06-06 11:58:44 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

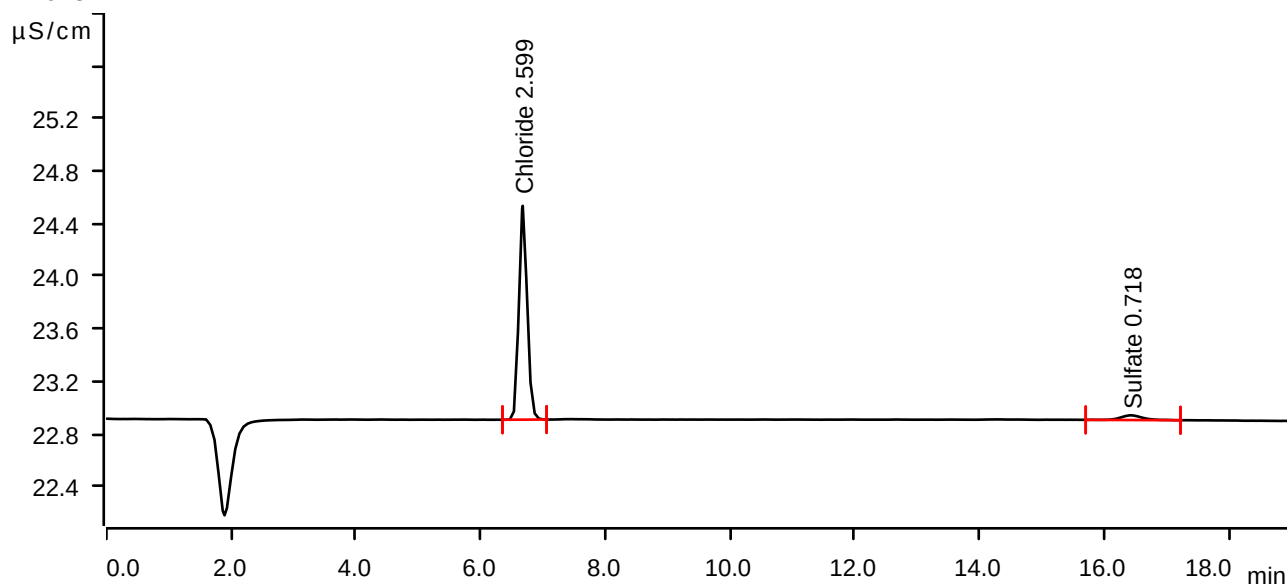

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	6.677	0.2508	1.628	2.599	Chloride
2	16.435	0.0146	0.036	0.718	Sulfate


Sample data

Ident P2749-07DLX10
Sample type Sample
Determination start 2024-06-06 12:20:18 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

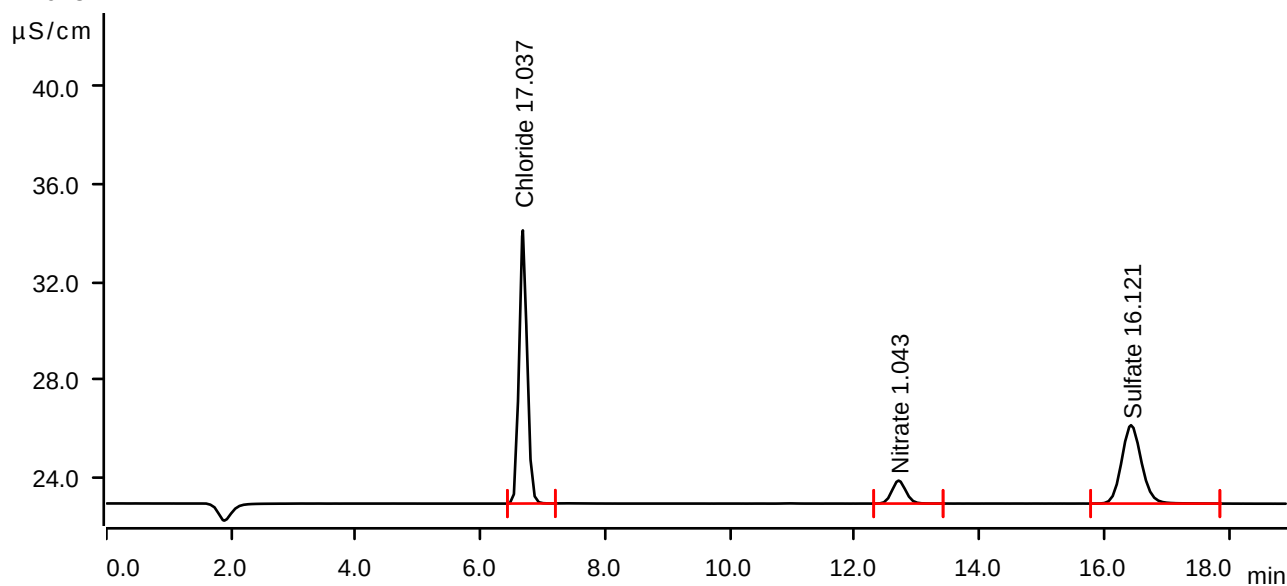

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.678	1.6709	11.199	17.037	Chloride
2	12.702	0.2448	0.943	1.043	Nitrate
3	16.428	1.1841	3.214	16.121	Sulfate


Sample data

Ident P2749-07DL2X100
Sample type Sample
Determination start 2024-06-06 12:41:52 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

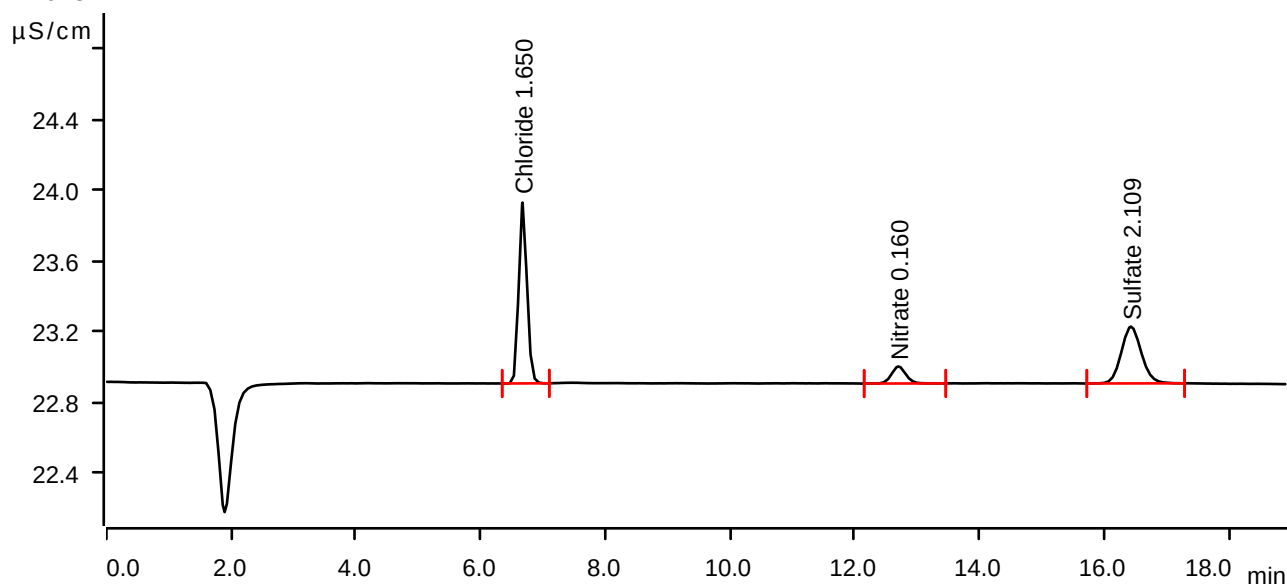

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.673	0.1574	1.024	1.650	Chloride
2	12.697	0.0259	0.097	0.160	Nitrate
3	16.427	0.1203	0.322	2.109	Sulfate


Sample data

Ident P2749-09DLX10
Sample type Sample
Determination start 2024-06-06 13:03:12 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

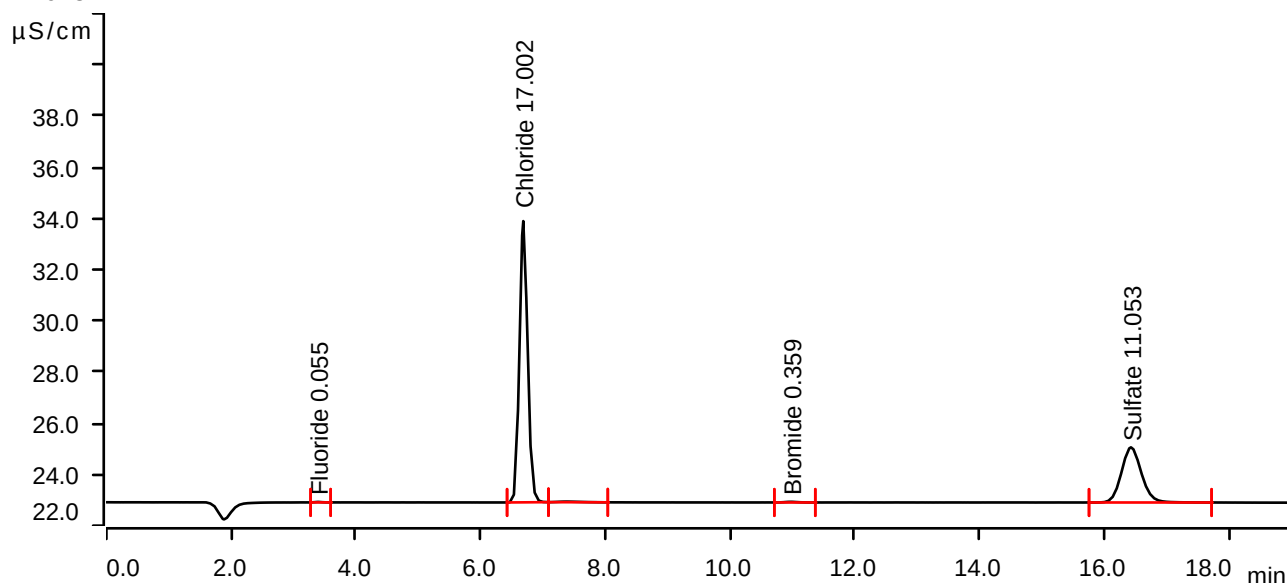

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0024	0.020	0.055	Fluoride
2	6.685	1.6675	10.982	17.002	Chloride
3	7.375	0.0099	0.023	invalid	
4	10.978	0.0058	0.025	0.359	Bromide
5	16.428	0.7993	2.154	11.053	Sulfate


Sample data

Ident P2749-09DL2X50
Sample type Sample
Determination start 2024-06-06 13:24:45 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

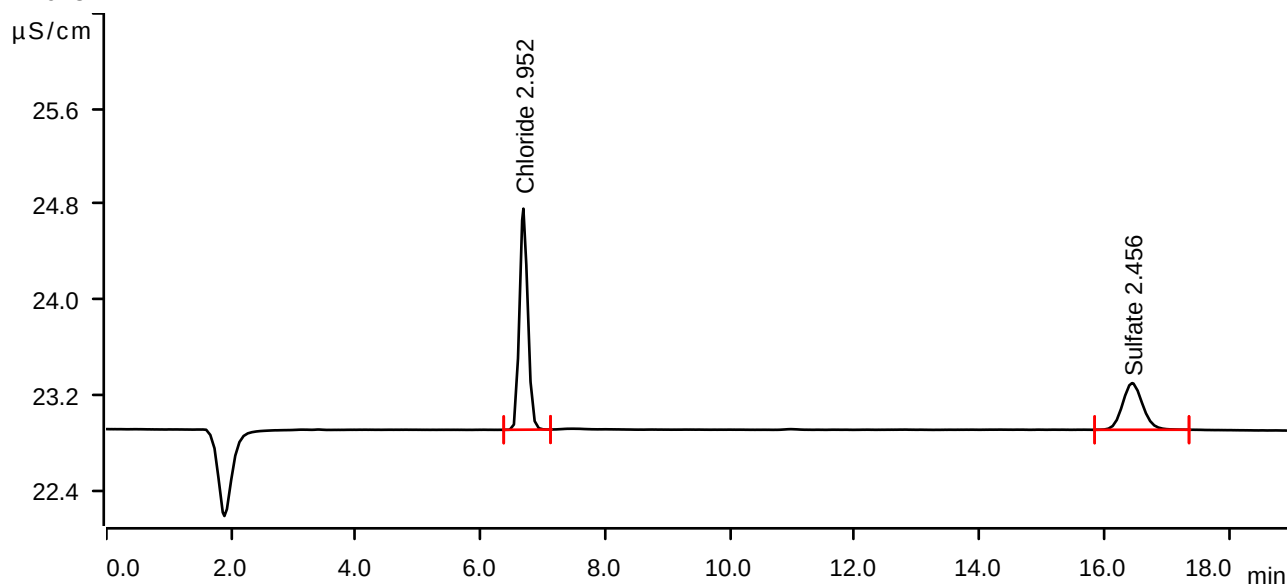

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.687	0.2855	1.855	2.952	Chloride
2	16.445	0.1466	0.392	2.456	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-06 13:46:17 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

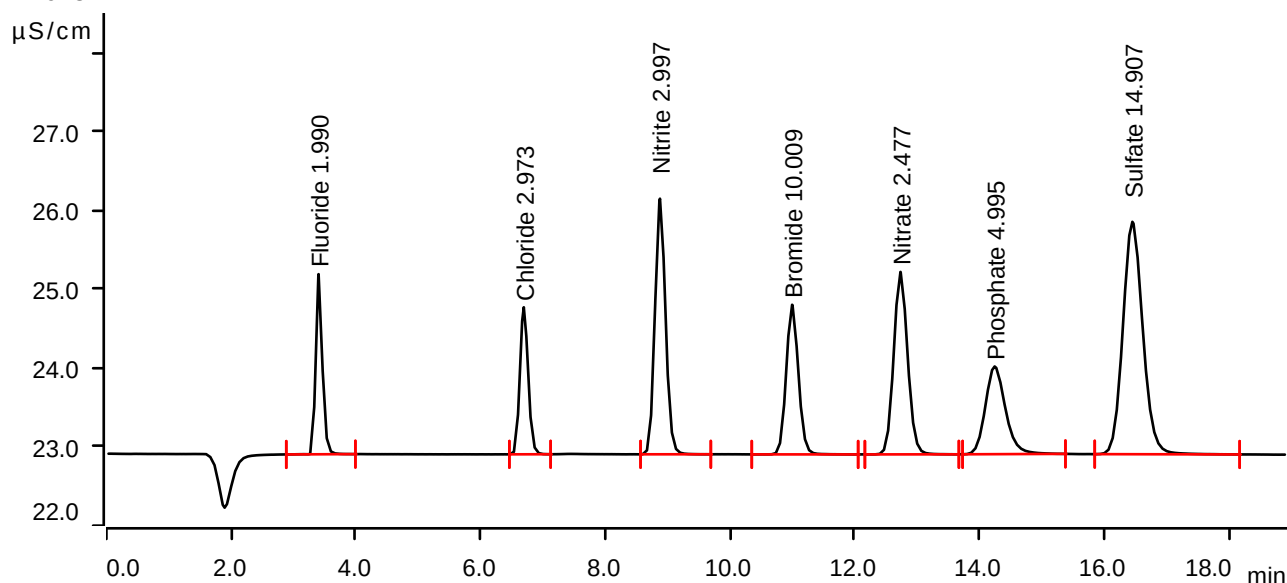


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.403	0.2840	2.286	1.990	Fluoride
2	6.693	0.2875	1.866	2.973	Chloride
3	8.877	0.6387	3.244	2.997	Nitrite
4	10.995	0.4303	1.899	10.009	Bromide
5	12.732	0.6001	2.315	2.477	Nitrate
6	14.242	0.4156	1.113	4.995	Phosphate
7	16.450	1.0919	2.949	14.907	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-06 14:07:47 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

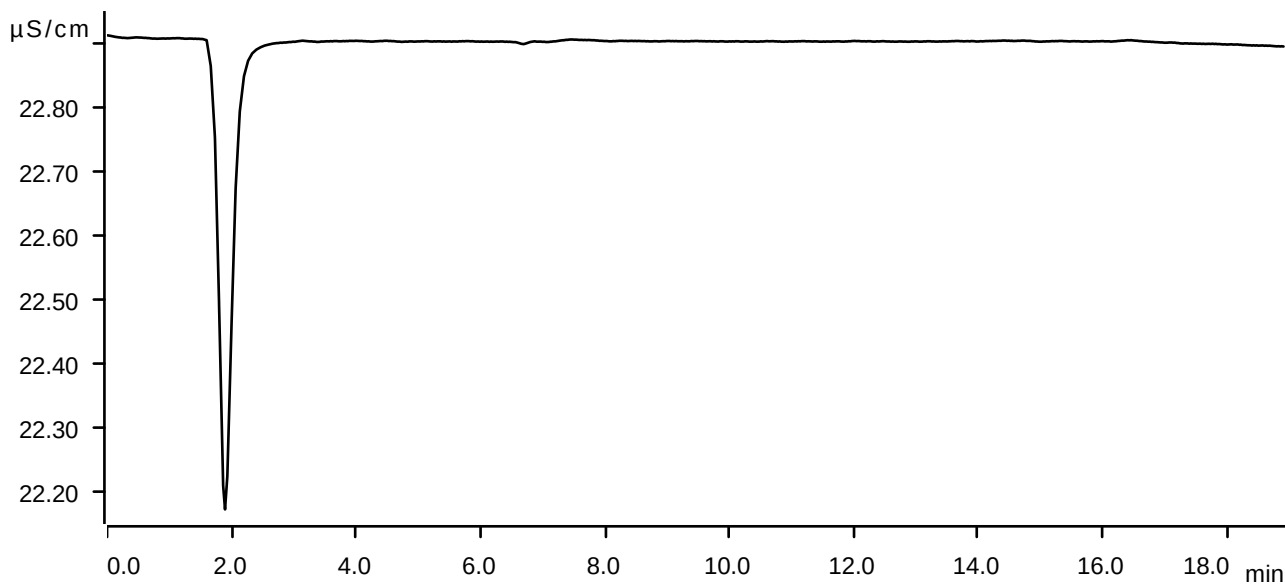Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-07 06:21:32 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

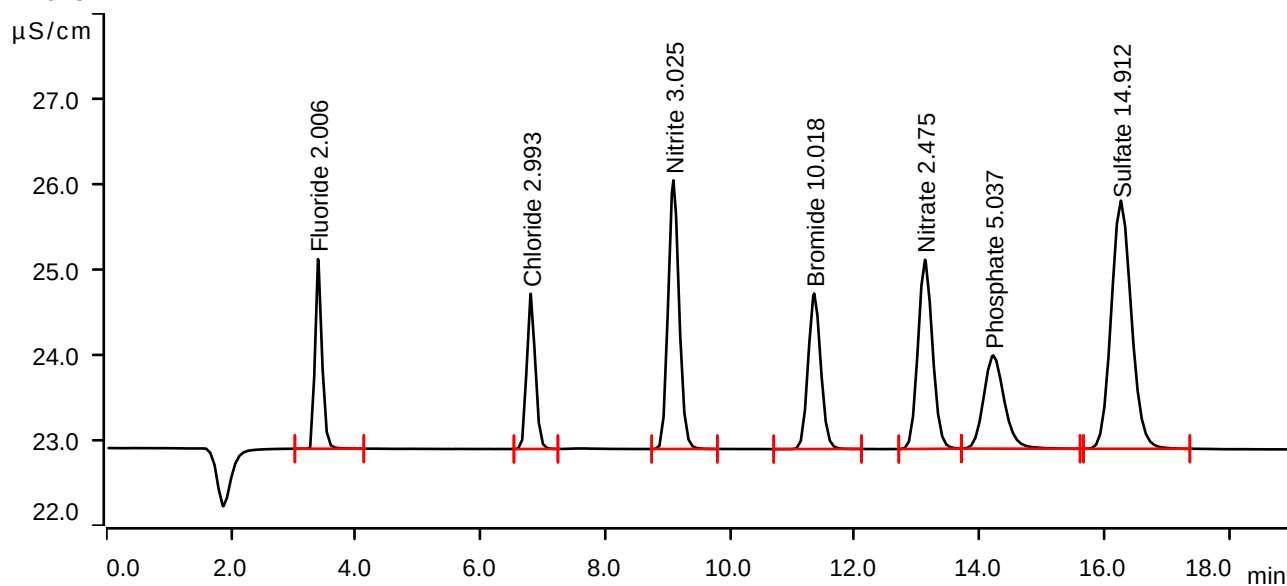

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2864	2.221	2.006	Fluoride
2	6.805	0.2895	1.819	2.993	Chloride
3	9.092	0.6449	3.147	3.025	Nitrite
4	11.350	0.4308	1.822	10.018	Bromide
5	13.125	0.5996	2.215	2.475	Nitrate
6	14.220	0.4192	1.092	5.037	Phosphate
7	16.265	1.0924	2.906	14.912	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-07 06:43:02 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

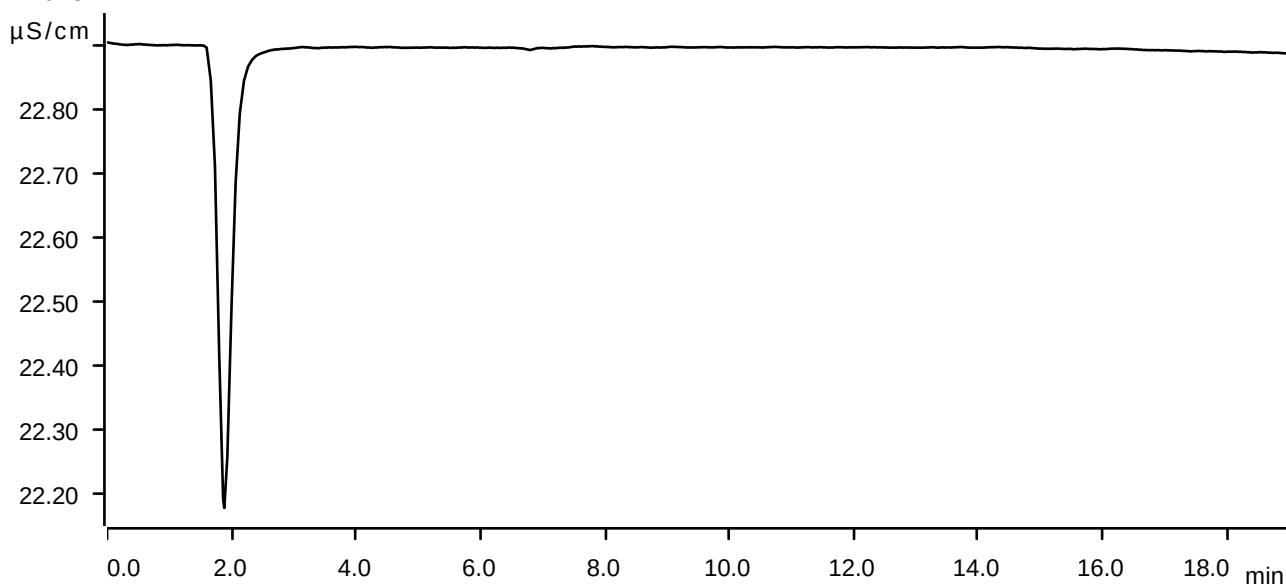


Sample data

Ident LB131125BLW3
 Sample type Sample
 Determination start 2024-06-07 07:04:32 UTC-4
 Method IC1-051324
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.56 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

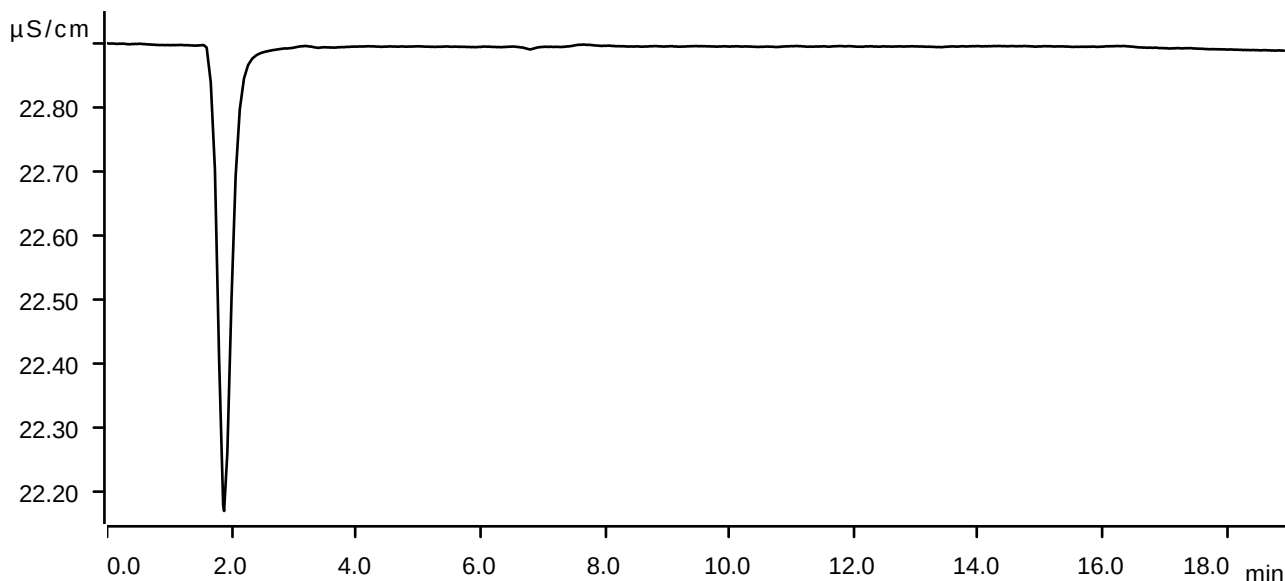


Sample data

Ident LB131125BSW3
Sample type Check standard 1
Determination start 2024-06-07 07:26:02 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

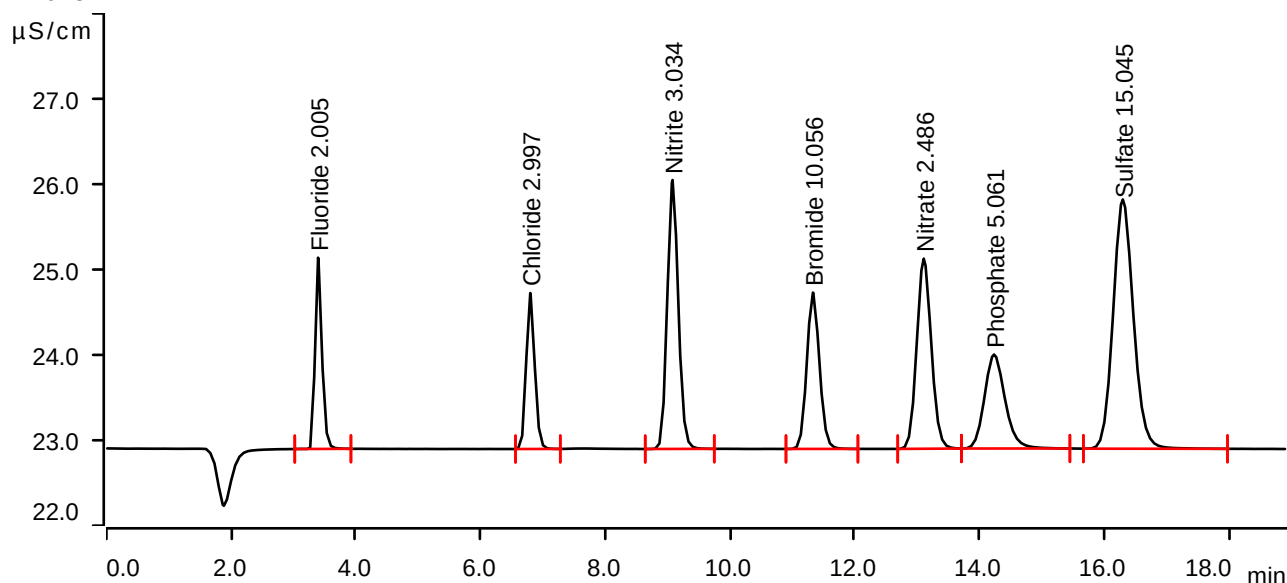

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.2863	2.241	2.005	Fluoride
2	6.797	0.2899	1.827	2.997	Chloride
3	9.078	0.6467	3.150	3.034	Nitrite
4	11.328	0.4324	1.831	10.056	Bromide
5	13.105	0.6024	2.227	2.486	Nitrate
6	14.232	0.4212	1.101	5.061	Phosphate
7	16.297	1.1024	2.920	15.045	Sulfate


Sample data

Ident P2749-03DL2X2
Sample type Sample
Determination start 2024-06-07 15:23:10 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

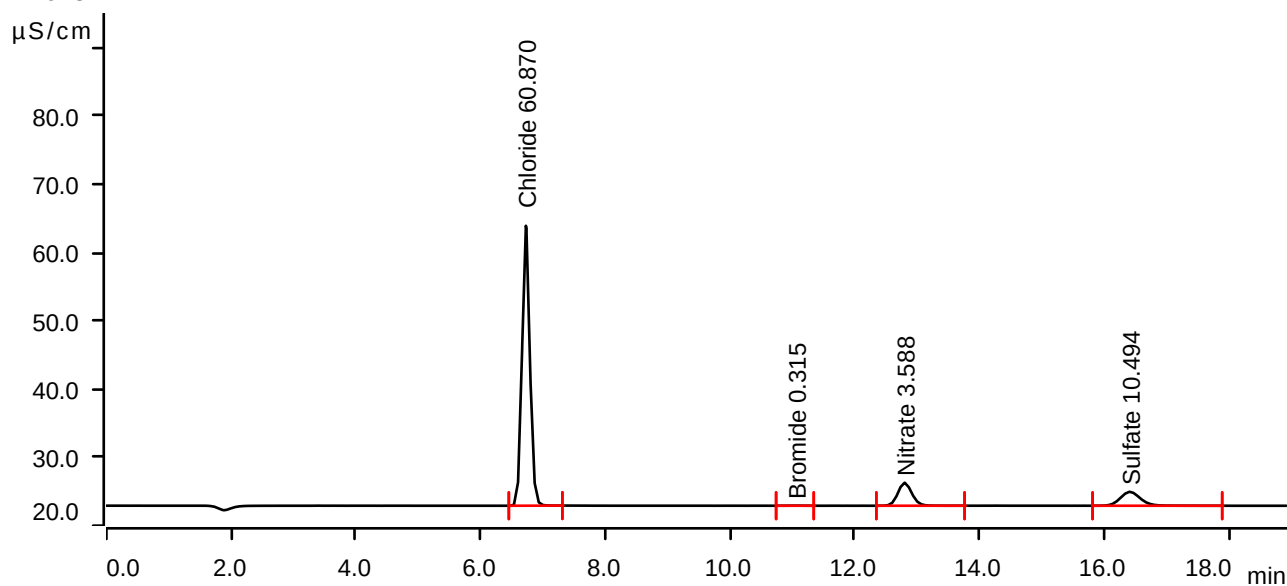

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.727	5.9824	40.986	60.870	Chloride
2	11.055	0.0038	0.017	0.315	Bromide
3	12.798	0.8754	3.369	3.588	Nitrate
4	16.408	0.7569	2.035	10.494	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-07 17:10:59 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

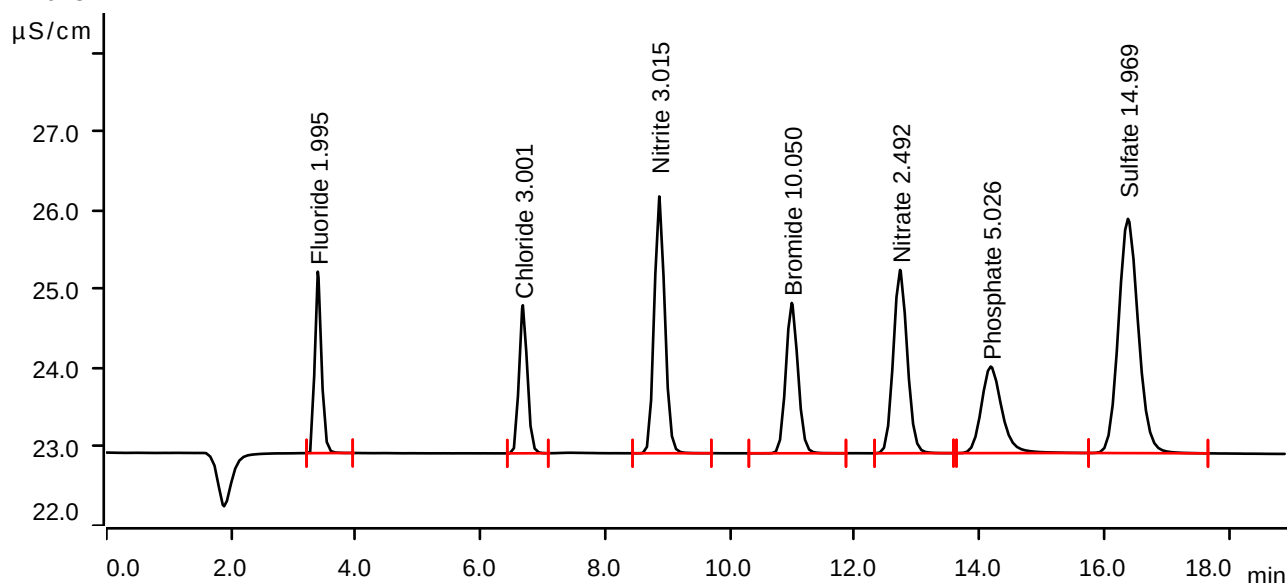


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.2848	2.303	1.995	Fluoride
2	6.678	0.2903	1.879	3.001	Chloride
3	8.865	0.6427	3.258	3.015	Nitrite
4	10.988	0.4322	1.908	10.050	Bromide
5	12.725	0.6039	2.326	2.492	Nitrate
6	14.178	0.4182	1.098	5.026	Phosphate
7	16.378	1.0966	2.973	14.969	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-07 17:32:29 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

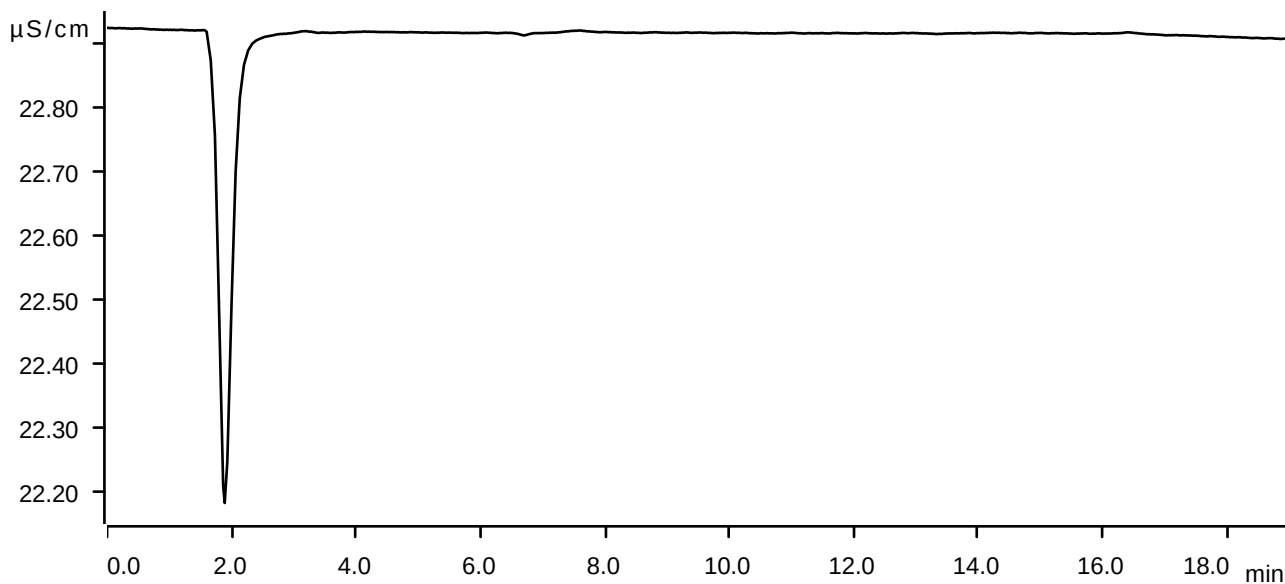Anions

WORKLIST(Hardcopy Internal Chain)

LB131125

WorkList Name : ANIONS - 06052024 WorkList ID : 180904 Department : Wet-Chemistry Date : 06-05-2024 14:12:04

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P2749-01	SY-10S	Water	Anions Group1	Cool 4 deg C	LOCK01	M21	06/04/2024	300.0
P2749-03	SY-10D	Water	Anions Group1	Cool 4 deg C	LOCK01	M21	06/04/2024	300.0
P2749-05	SY-10I	Water	Anions Group1	Cool 4 deg C	LOCK01	M21	06/04/2024	300.0
P2749-07	SY-12D	Water	Anions Group1	Cool 4 deg C	LOCK01	M21	06/04/2024	300.0
P2749-09	SY-12I	Water	Anions Group1	Cool 4 deg C	LOCK01	M21	06/04/2024	300.0

Date/Time 06.05.2024, 16:50
Raw Sample Received by: NF(wc)
Raw Sample Relinquished by: [Signature]

Date/Time 06.05.2024, 17:30
Raw Sample Received by: [Signature]
Raw Sample Relinquished by: NF(wc)