

6137366

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

9/30/2025 12:21

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.358	0.0	0.085	
ICB1	0.631	0.0	0.001	
CCV1	242.934	0.0	0.215	
CCB1	0.751	0.0	0.001	
PB169885BL	0.767	0.0	0.001	
Q3215-01	0.690	0.0	0.001	
Q3215-01DUP	0.469	0.0	0.001	
Q3231-04	0.540	0.0	0.001	
Q3231-08	0.796	0.0	0.001	
Q3231-12	0.541	0.0	0.001	
Q3231-16	0.761	0.0	0.001	
Q3233-01	0.585	0.0	0.001	
CCV2	245.150	0.0	0.217	
CCB2	1.088	0.0	0.001	

N 14
Mean 42.290
SD 89.1703
CV% 210.85

Aquakem v. 7.2AQ1

Results from time period:

Tue Sep 30 12:12:55 2025

Tue Sep 30 12:20:11 2025

Sample Id	Sam/Ctr/c	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.4719	µg/l	9/30/2025 9:05:32	
5.0PPBCN	A	Total CN	P	5.61	µg/l	9/30/2025 9:05:33	
10PPBCN	A	Total CN	P	10.4396	µg/l	9/30/2025 9:05:34	
50PPBCN	A	Total CN	P	47.8297	µg/l	9/30/2025 9:05:35	
100PPBCN	A	Total CN	P	100.8495	µg/l	9/30/2025 9:05:36	
250PPBCN	A	Total CN	P	249.5344	µg/l	9/30/2025 9:05:37	
500PPBCN	A	Total CN	P	500.2651	µg/l	9/30/2025 9:05:38	
ICV1	S	Total CN	P	96.3578	µg/l	9/30/2025 12:12:55	
ICB1	S	Total CN	P	0.6315	µg/l	9/30/2025 12:12:57	
CCV1	S	Total CN	P	242.934	µg/l	9/30/2025 12:13:00	
CCB1	S	Total CN	P	0.751	µg/l	9/30/2025 12:13:01	
PB169885BL	S	Total CN	P	0.7673	µg/l	9/30/2025 12:13:04	
Q3215-01	S	Total CN	P	0.6904	µg/l	9/30/2025 12:13:05	
Q3215-01DUP	S	Total CN	P	0.4686	µg/l	9/30/2025 12:20:02	
Q3231-04	S	Total CN	P	0.54	µg/l	9/30/2025 12:20:03	
Q3231-08	S	Total CN	P	0.7961	µg/l	9/30/2025 12:20:04	
Q3231-12	S	Total CN	P	0.541	µg/l	9/30/2025 12:20:05	
Q3231-16	S	Total CN	P	0.7609	µg/l	9/30/2025 12:20:06	
Q3233-01	S	Total CN	P	0.5847	µg/l	9/30/2025 12:20:07	
CCV2	S	Total CN	P	245.1498	µg/l	9/30/2025 12:20:10	
CCB2	S	Total CN	P	1.0877	µg/l	9/30/2025 12:20:11	

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

9/30/2025 9:06


Test Total CN

Accepted 9/30/2025 9:05

Factor 1131
Bias 0

Coeff. of det. 0.999968

Errors

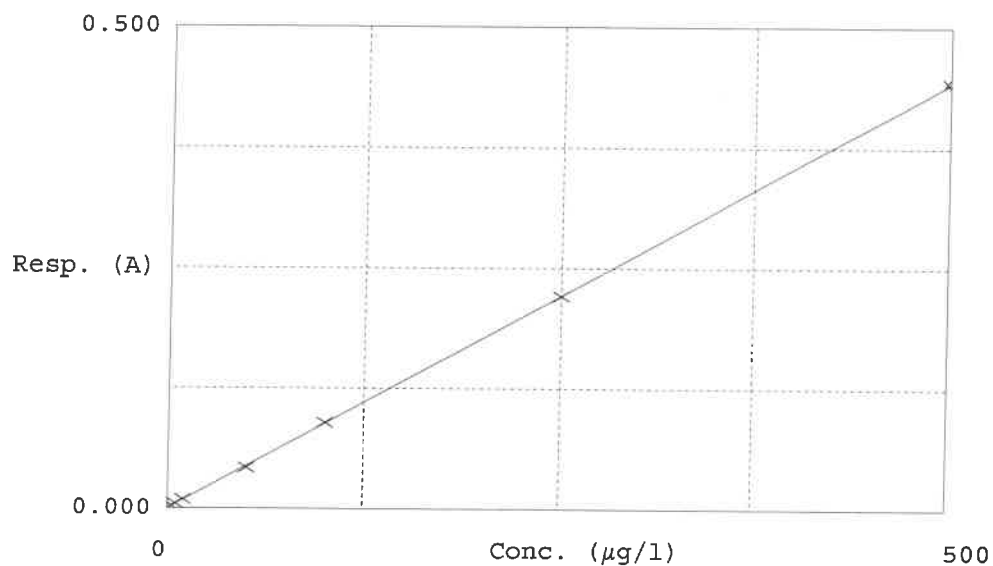

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.0PPBCN	0.001	0.4719	0.0000	✓
2	5.0PPBCN	0.005	5.6100	5.0000	12.2
3	10PPBCN	0.009	10.4396	10.0000	4.4
4	50PPBCN	0.042	47.8297	50.0000	4.3
5	100PPBCN	0.089	100.8495	100.0000	0.8
6	250PPBCN	0.221	249.5344	250.0000	-0.2
7	500PPBCN	0.443	500.2651	500.0000	0.1

09/30/2025
RM