

66137517

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

10/14/2025 11:18

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.907	0.0	0.087	
ICB1	0.629	0.0	0.001	
CCV1	236.260	0.0	0.213	
CCB1	0.777	0.0	0.001	
RL CHECK	4.649	0.0	0.004	
PB170085BL	0.497	0.0	0.001	
PB170085BS	96.548	0.0	0.087	
MIDPB170085	238.203	0.0	0.215	
Q3258-08	3.336	0.0	0.003	
Q3258-08DUP	3.381	0.0	0.003	
Q3258-09	3.519	0.0	0.003	
CCV2	244.830	0.0	0.220	
CCB2	0.872	0.0	0.001	

93% (50-150)

10/14/2025

RM

95% (90-110)

N 13
Mean 71.493
SD 101.9123
CV% 142.55

Aquakem v. 7.2AQ1

Results from time period:

Tue Oct 14 10:44:54 2025

Tue Oct 14 11:18:09 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.2291	µg/l	10/14/2025 9:13:26	
5.0PPBCN	A	Total CN	P	5.3249	µg/l	10/14/2025 9:13:27	
10PPBCN	A	Total CN	P	10.1874	µg/l	10/14/2025 9:13:28	
50PPBCN	A	Total CN	P	48.0572	µg/l	10/14/2025 9:13:29	
100PPBCN	A	Total CN	P	102.1669	µg/l	10/14/2025 9:13:30	
250PPBCN	A	Total CN	P	248.5611	µg/l	10/14/2025 9:13:31	
500PPBCN	A	Total CN	P	500.4734	µg/l	10/14/2025 9:13:32	
ICV1	S	Total CN	P	95.9068	µg/l	10/14/2025 10:44:54	
ICB1	S	Total CN	P	0.6288	µg/l	10/14/2025 10:44:56	
CCV1	S	Total CN	P	236.2605	µg/l	10/14/2025 10:44:59	
CCB1	S	Total CN	P	0.7775	µg/l	10/14/2025 10:45:01	
RL CHECK	S	Total CN	P	4.6494	µg/l	10/14/2025 10:52:29	
PB170085BL	S	Total CN	P	0.4973	µg/l	10/14/2025 10:52:30	
PB170085BS	S	Total CN	P	96.5475	µg/l	10/14/2025 10:52:33	
MIDPB170085	S	Total CN	P	238.2027	µg/l	10/14/2025 10:52:35	
Q3258-08	S	Total CN	P	3.3358	µg/l	10/14/2025 11:18:02	
Q3258-08DUP	S	Total CN	P	3.381	µg/l	10/14/2025 11:18:04	
Q3258-09	S	Total CN	P	3.5186	µg/l	10/14/2025 11:18:06	
CCV2	S	Total CN	P	244.8302	µg/l	10/14/2025 11:18:08	
CCB2	S	Total CN	P	0.8723	µg/l	10/14/2025 11:18:09	

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

10/14/2025 9:13


Test Total CN

Accepted 10/14/2025 9:13

Factor 1112
Bias 0

Coeff. of det. 0.999947

Errors

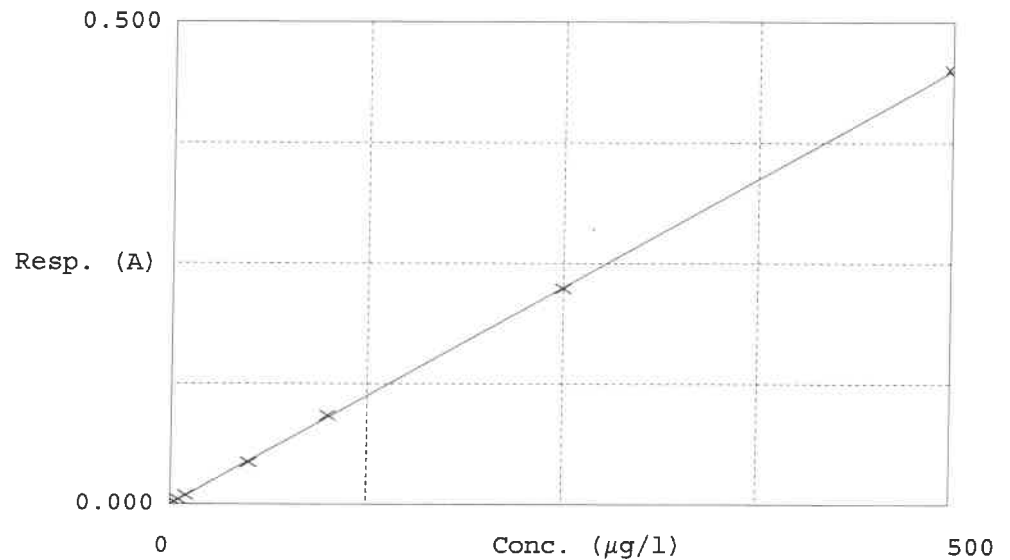

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.2291	0.0000	-
2	5.0PPBCN	0.005	5.3249	5.0000	6.5
3	10PPBCN	0.009	10.1874	10.0000	1.9
4	50PPBCN	0.044	48.0572	50.0000	-3.9
5	100PPBCN	0.092	102.1669	100.0000	
6	250PPBCN	0.224	248.5611	250.0000	2.2
7	500PPBCN	0.450	500.4734	500.0000	-0.6 0.1

10/14/2025
RM