

66137590

=====

Test results	Aquakem 7.2AQ1	Page: 1
--------------	----------------	---------

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

10/21/2025 11:31

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.098	0.0	0.081	
ICB1	0.150	0.0	0.001	
CCV1	237.663	0.0	0.206	
CCB1	0.424	0.0	0.001	
PB170154BL	0.468	0.0	0.001	
PB170154BS	97.066	0.0	0.084	
LOWPB170154	10.525	0.0	0.010	
HIGHPB170154	508.188	0.0	0.440	
Q3367-01	0.617	0.0	0.001	
Q3367-01DUP	0.549	0.0	0.001	
Q3367-01MS	46.497	0.0	0.041	
Q3367-01MSD	47.494	0.0	0.042	
CCV2	257.172	0.0	0.223	
CCB2	0.533	0.0	0.001	

105% (90-110) 10/21/2025
102% (90-110) RM

N	14
Mean	92.889
SD	147.4653
CV%	158.75

Aquakem v. 7.2AQ1

Results from time period:

Tue Oct 21 08:44:26 2025

Tue Oct 21 11:29:49 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.1297	µg/l	10/21/2025 10:18:49	
5.0PPBCN	A	Total CN	P	5.0315	µg/l	10/21/2025 10:18:50	
10PPBCN	A	Total CN	P	10.2776	µg/l	10/21/2025 10:18:51	
50PPBCN	A	Total CN	P	49.3188	µg/l	10/21/2025 10:18:52	
100PPBCN	A	Total CN	P	99.598	µg/l	10/21/2025 10:18:53	
250PPBCN	A	Total CN	P	251.0035	µg/l	10/21/2025 10:18:54	
500PPBCN	A	Total CN	P	499.6409	µg/l	10/21/2025 10:18:55	
ICV1	S	Total CN	P	93.0981	µg/l	10/21/2025 10:53:23	
ICB1	S	Total CN	P	0.1502	µg/l	10/21/2025 10:53:24	
CCV1	S	Total CN	P	237.6634	µg/l	10/21/2025 10:53:27	
CCB1	S	Total CN	P	0.4242	µg/l	10/21/2025 10:53:29	
PB170154BL	S	Total CN	P	0.4685	µg/l	10/21/2025 10:53:31	
PB170154BS	S	Total CN	P	97.0657	µg/l	10/21/2025 10:58:09	
LOWPB170154	S	Total CN	P	10.525	µg/l	10/21/2025 10:58:10	
HIGHPB170154	S	Total CN	P	508.1877	µg/l	10/21/2025 11:04:13	
Q3367-01	S	Total CN	P	0.6168	µg/l	10/21/2025 11:04:15	
Q3367-01DUP	S	Total CN	P	0.5489	µg/l	10/21/2025 11:04:16	
Q3367-01MS	S	Total CN	P	46.4966	µg/l	10/21/2025 11:29:46	
Q3367-01MSD	S	Total CN	P	47.4938	µg/l	10/21/2025 11:29:47	
CCV2	S	Total CN	P	257.1718	µg/l	10/21/2025 11:29:48	
CCB2	S	Total CN	P	0.5327	µg/l	10/21/2025 11:29:49	

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

10/21/2025 10:21


Test Total CN

Accepted 10/21/2025 10:21

Factor 1156
Bias 0

Coeff. of det. 0.999991

Errors

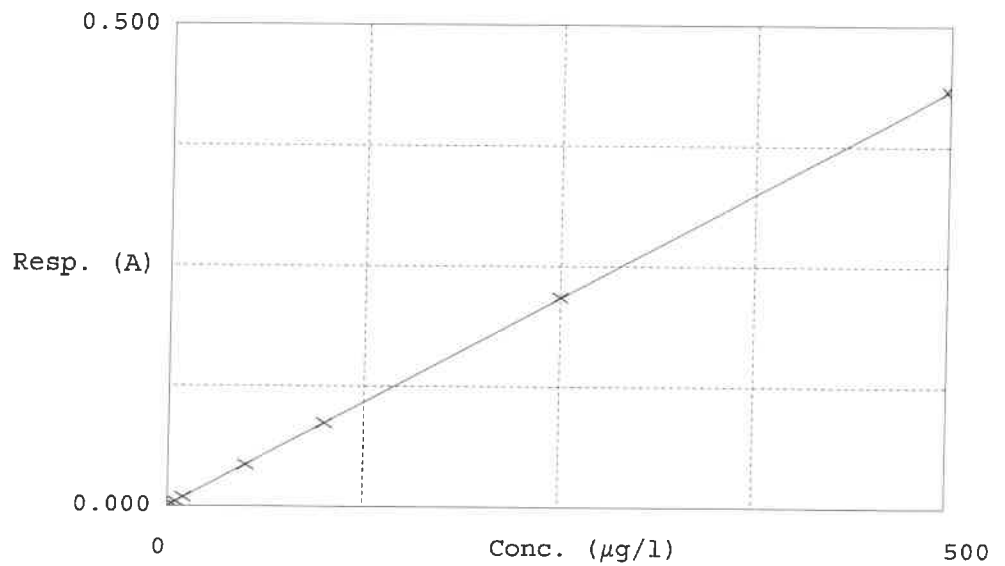

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.0PPBCN	0.001	0.1297	0.0000	-
2	5.0PPBCN	0.005	5.0315	5.0000	0.6
3	10PPBCN	0.009	10.2776	10.0000	2.8
4	50PPBCN	0.043	49.3188	50.0000	-1.4
5	100PPBCN	0.087	99.5980	100.0000	-0.4
6	250PPBCN	0.218	251.0035	250.0000	0.4
7	500PPBCN	0.433	499.6409	500.0000	-0.1

10/21/2025
RM