

66137920

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

11/17/2025 17:15

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.003	0.0	0.107	
ICB1	0.015	0.0	0.008	
CCV1	0.966	0.0	0.103	
CCB1	0.009	0.0	0.007	
PB170568BL	0.016	0.0	0.008	
PB170568BS	1.003	0.0	0.107	
Q3530-01	0.033	0.0	0.010	
Q3530-02	0.056	0.0	0.012	
PB170567BL	0.011	0.0	0.007	
PB170567BS	1.003	0.0	0.107	
Q3530-07	0.037	0.0	0.010	
Q3530-08	0.056	0.0	0.012	
CCV2	0.980	0.0	0.105	
CCB2	0.011	0.0	0.007	

N 14
Mean 0.371
SD 0.4797
CV% 129.20

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 17 17:04:00 2025

Mon Nov 17 17:14:05 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0005	mg/l	11/17/2025 15:46:38	
0.05PPM	A	Phenolics-	P	0.0582	mg/l	11/17/2025 15:46:39	
0.1PPM	A	Phenolics-	P	0.1053	mg/l	11/17/2025 15:46:40	
0.25PPM	A	Phenolics-	P	0.251	mg/l	11/17/2025 15:46:41	
0.50PPM	A	Phenolics-	P	0.4996	mg/l	11/17/2025 15:46:42	
1.0PPM	A	Phenolics-	P	0.9739	mg/l	11/17/2025 15:46:43	
2.0PPM	A	Phenolics-	P	2.0125	mg/l	11/17/2025 15:46:44	
ICV1	S	Phenolics-	P	1.0026	mg/l	11/17/2025 17:04:00	
ICB1	S	Phenolics-	P	0.0146	mg/l	11/17/2025 17:04:02	
CCV1	S	Phenolics-	P	0.9661	mg/l	11/17/2025 17:04:04	
CCB1	S	Phenolics-	P	0.0095	mg/l	11/17/2025 17:04:06	
PB170568BL	S	Phenolics-	P	0.0159	mg/l	11/17/2025 17:04:08	
PB170568BS	S	Phenolics-	P	1.0032	mg/l	11/17/2025 17:04:11	
Q3530-01	S	Phenolics-	P	0.0328	mg/l	11/17/2025 17:13:55	
Q3530-02	S	Phenolics-	P	0.0559	mg/l	11/17/2025 17:13:57	
PB170567BL	S	Phenolics-	P	0.0108	mg/l	11/17/2025 17:13:58	
PB170567BS	S	Phenolics-	P	1.0032	mg/l	11/17/2025 17:13:59	
Q3530-07	S	Phenolics-	P	0.037	mg/l	11/17/2025 17:14:00	
Q3530-08	S	Phenolics-	P	0.0559	mg/l	11/17/2025 17:14:01	
CCV2	S	Phenolics-	P	0.9796	mg/l	11/17/2025 17:14:03	
CCB2	S	Phenolics-	P	0.0106	mg/l	11/17/2025 17:14:05	

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

11/17/2025 15:48


Test Phenolics-

Accepted 11/17/2025 15:48

Factor 9.96
Bias 0.006

Coeff. of det. 0.999704

Errors

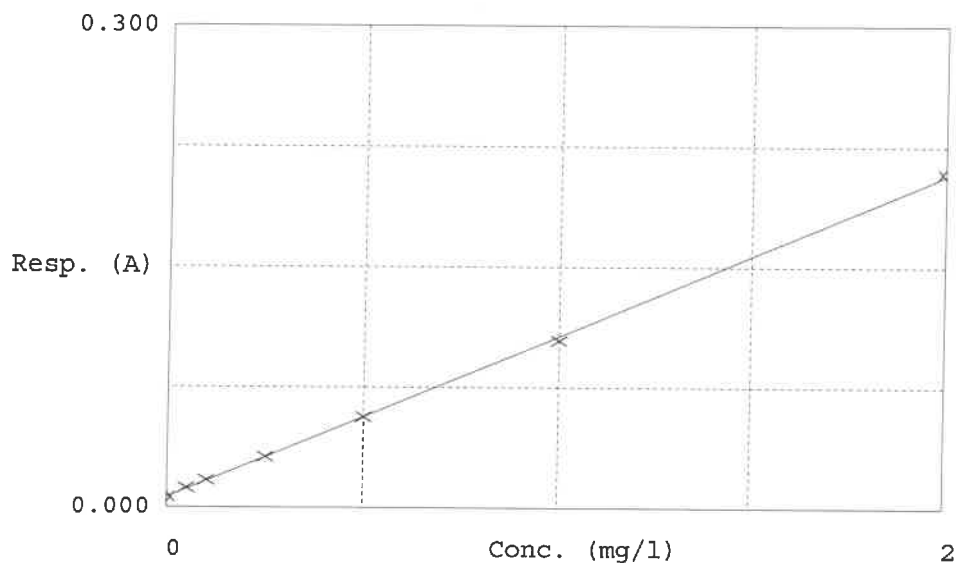

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	-0.0005	0.0000	-
2	Phenol-2	0.012	0.0582	0.0500	16.4
3	Phenol-2	0.017	0.1053	0.1000	5.3
4	Phenol-2	0.032	0.2510	0.2500	0.4
5	Phenol-2	0.057	0.4996	0.5000	-0.1
6	Phenol-2	0.104	0.9739	1.0000	-2.6
7	Phenol-2	0.208	2.0125	2.0000	0.6

11/17/2025
RM