

0885158

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

1/3/2017 14:40

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	99.802	0.0	0.095	
ICB1	-0.176	0.0	0.005	
CCV1	247.625	0.0	0.229	
CCB1	1.786	0.0	0.007	
LOWPB95735	9.521	0.0	0.014	
HIGHPB95735	498.959	0.0	0.456	
PB95735BLS	0.509	0.0	0.006	
PB95735BSS	102.056	0.0	0.097	
H6322-03	1.580	0.0	0.007	
H6322-03D	1.073	0.0	0.006	
H6322-03S	3.213	0.0	0.008	
H6322-03SD	4.098	0.0	0.009	
CCV2	268.700	0.0	0.248	
CCB2	-0.283	0.0	0.005	

N	14
Mean	88.462
SD	150.2363
CV%	169.83

Aquakem v. 7.2AQ1

Results from time period:

Tue Jan 03 14:07:23 2017

21K

Tue Jan 03 14:32:24 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.1962	µg/l	1/3/2017 12:43:29	
5.OPPBCN	A	Total CN	P	4.9261	µg/l	1/3/2017 12:43:30	
10PPBCN	A	Total CN	P	11.5016	µg/l	1/3/2017 12:43:31	
50PPBCN	A	Total CN	P	49.453	µg/l	1/3/2017 12:43:32	
100PPBCN	A	Total CN	P	100.3035	µg/l	1/3/2017 12:43:33	
250PPBCN	A	Total CN	P	248.0946	µg/l	1/3/2017 12:43:34	
500PPBCN	A	Total CN	P	500.9174	µg/l	1/3/2017 12:43:35	
ICV1	S	Total CN	P	99.8024	µg/l	1/3/2017 14:07:23	
ICB1	S	Total CN	P	-0.176	µg/l	1/3/2017 14:07:24	
CCV1	S	Total CN	P	247.6253	µg/l	1/3/2017 14:07:25	
CCB1	S	Total CN	P	1.7864	µg/l	1/3/2017 14:07:26	
LOWPB95735	S	Total CN	P	9.5213	µg/l	1/3/2017 14:07:27	
HIGHPB95735	S	Total CN	P	498.9591	µg/l	1/3/2017 14:07:28	
PB95735BLS	S	Total CN	P	0.509	µg/l	1/3/2017 14:07:29	
PB95735BSS	S	Total CN	P	102.0558	µg/l	1/3/2017 14:07:30	
H6322-03	S	Total CN	P	1.5804	µg/l	1/3/2017 14:07:31	
H6322-03D	S	Total CN	P	1.0725	µg/l	1/3/2017 14:07:32	
H6322-03S	S	Total CN	P	3.2131	µg/l	1/3/2017 14:32:21	
H6322-03SD	S	Total CN	P	4.0984	µg/l	1/3/2017 14:32:22	
CCV2	S	Total CN	P	268.7002	µg/l	1/3/2017 14:32:23	
CCB2	S	Total CN	P	-0.2834	µg/l	1/3/2017 14:32:24	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

1/3/2017 12:58


Test Total CN

Accepted 1/3/2017 12:58

Factor 1106
Bias 0.005

Coeff. of det. 0.999965

Errors

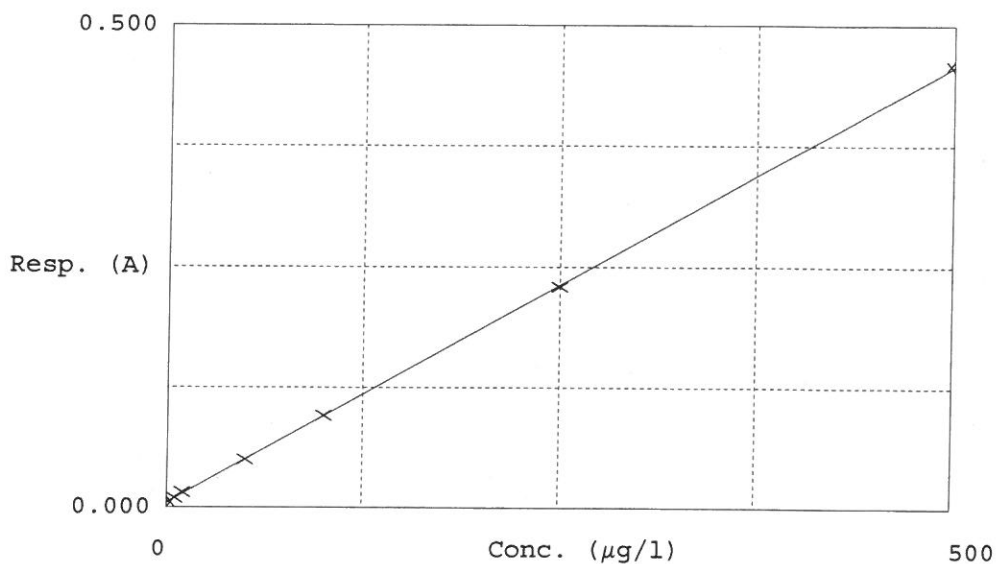

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.005	-0.1962	0.0000	
2	5.0PPBCN	0.010	4.9261	5.0000	
3	10PPBCN	0.016	11.5016	10.0000	
4	50PPBCN	0.050	49.4530	50.0000	
5	100PPBCN	0.096	100.3035	100.0000	
6	250PPBCN	0.229	248.0946	250.0000	
7	500PPBCN	0.458	500.9174	500.0000	