

685286

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AK

1/11/2017 13:45

Test: Reactive AK 11/11/17
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.872	0.0	0.094	
ICB1	1.195	0.0	0.004	
CCV1	234.327	0.0	0.225	
CCB1	3.216	0.0	0.006	
PB95864BLS	1.382	0.0	0.005	
I1078-02	1.164	0.0	0.004	
I1078-02D	2.965	0.0	0.006	
I1079-02	1.139	0.0	0.004	
PB95920BLS	1.684	0.0	0.005	
I1098-05	1.001	0.0	0.004	
I1098-05D	0.848	0.0	0.004	
CCV2	242.312	0.0	0.232	
CCB2	1.666	0.0	0.005	

N 13
Mean 45.290
SD 89.5279
CV% 197.68

LB85-286

Aquakem v. 7.2AQ1

Results from time period:

Wed Jan 11 13:11:59 2017

Wed Jan 11 13:36:32 2017

AK

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.9387	µg/l	1/11/2017 10:40:32	
5.OPPBCN	A	Reactive CN	P	6.0955	µg/l	1/11/2017 10:40:33	
10PPBCN	A	Reactive CN	P	10.3316	µg/l	1/11/2017 10:40:34	
50PPBCN	A	Reactive CN	P	53.3626	µg/l	1/11/2017 10:40:35	
100PPBCN	A	Reactive CN	P	99.5482	µg/l	1/11/2017 10:40:36	
250PPBCN	A	Reactive CN	P	239.9739	µg/l	1/11/2017 10:40:37	
500PPBCN	A	Reactive CN	P	504.7496	µg/l	1/11/2017 10:40:38	
ICV1	S	Reactive CN	P	95.872	µg/l	1/11/2017 13:11:59	
ICB1	S	Reactive CN	P	1.1948	µg/l	1/11/2017 13:12:00	
CCV1	S	Reactive CN	P	234.3268	µg/l	1/11/2017 13:12:01	
CCB1	S	Reactive CN	P	3.2159	µg/l	1/11/2017 13:12:02	
PB95864BLS	S	Reactive CN	P	1.3816	µg/l	1/11/2017 13:12:03	
I1078-02	S	Reactive CN	P	1.1636	µg/l	1/11/2017 13:12:04	
I1078-02D	S	Reactive CN	P	2.965	µg/l	1/11/2017 13:12:05	
I1079-02	S	Reactive CN	P	1.1387	µg/l	1/11/2017 13:12:06	
PB95920BLS	S	Reactive CN	P	1.6838	µg/l	1/11/2017 13:12:07	
I1098-05	S	Reactive CN	P	1.001	µg/l	1/11/2017 13:12:08	
I1098-05D	S	Reactive CN	P	0.8478	µg/l	1/11/2017 13:12:09	
CCV2	S	Reactive CN	P	242.3123	µg/l	1/11/2017 13:15:22	
CCB2	S	Reactive CN	P	1.666	µg/l	1/11/2017 13:15:23	

LB 85286

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

1/11/2017 10:43


Test Total CN

Accepted 1/11/2017 10:43

Factor 1059
Bias 0.003

Coeff. of det. 0.999335

Errors

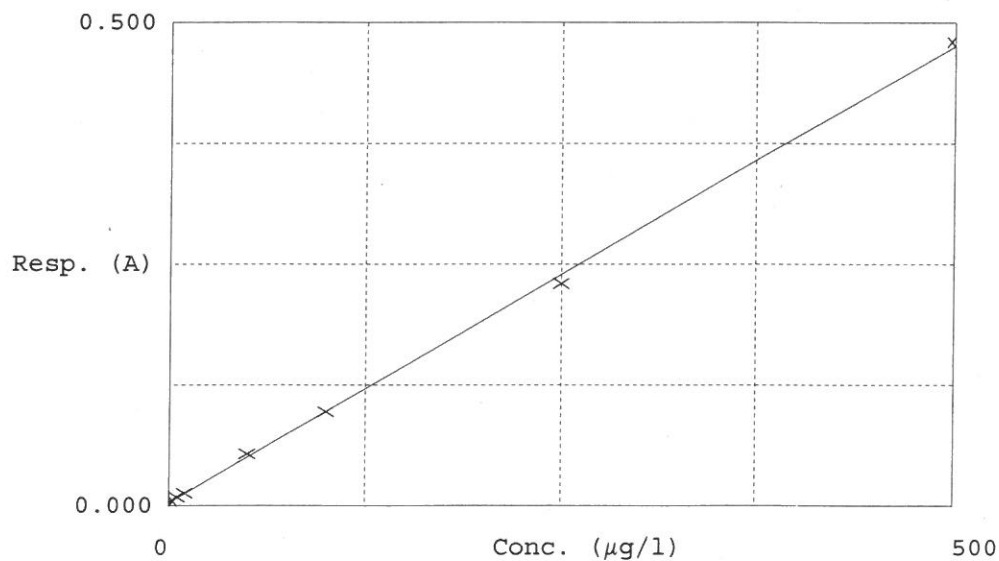

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.9387	0.0000	
2	5.0PPBCN	0.009	6.0955	5.0000	
3	10PPBCN	0.013	10.3316	10.0000	
4	50PPBCN	0.054	53.3626	50.0000	
5	100PPBCN	0.097	99.5482	100.0000	
6	250PPBCN	0.230	239.9739	250.0000	
7	500PPBCN	0.480	504.7496	500.0000	