

LB25853

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

2/16/2017 14:10

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.913	0.0	0.105	
ICB1	-0.004	0.0	0.005	
CCV1	0.984	0.0	0.113	
CCB1	-0.009	0.0	0.005	
PB96970BLS	-0.004	0.0	0.005	
PB96970BSS	0.919	0.0	0.105	
I1826-03	-0.002	0.0	0.005	
I1826-03D	-0.007	0.0	0.005	
I1826-03S	0.882	0.0	0.101	
I1826-03SD	0.887	0.0	0.102	
I1850-05	-0.001	0.0	0.005	
CCV2	0.979	0.0	0.112	
CCB2	-0.004	0.0	0.005	

N	13
Mean	0.426
SD	0.4843
CV%	113.80

LB85853

Aquakem v. 7.2AQ1

Results from time period:

Thu Feb 16 13:36:03 2017

Aik

Thu Feb 16 14:09:27 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0497	mg/l	2/16/2017 13:36:03	
0.1PPM	A	Phenolics-	P	0.0978	mg/l	2/16/2017 13:36:04	
0.25PPM	A	Phenolics-	P	0.2541	mg/l	2/16/2017 13:36:05	
0.50PPM	A	Phenolics-	P	0.4972	mg/l	2/16/2017 13:36:06	
1.0PPM	A	Phenolics-	P	1.0018	mg/l	2/16/2017 13:36:07	
2.0PPM	A	Phenolics-	P	1.9994	mg/l	2/16/2017 13:36:08	
ICV1	S	Phenolics-	P	0.9128	mg/l	2/16/2017 14:05:28	
ICB1	S	Phenolics-	P	-0.004	mg/l	2/16/2017 14:05:29	
CCV1	S	Phenolics-	P	0.9841	mg/l	2/16/2017 14:05:30	
CCB1	S	Phenolics-	P	-0.0085	mg/l	2/16/2017 14:05:31	
PB96970BLS	S	Phenolics-	P	-0.0044	mg/l	2/16/2017 14:05:32	
PB96970BSS	S	Phenolics-	P	0.9194	mg/l	2/16/2017 14:05:33	
I1826-03	S	Phenolics-	P	-0.0024	mg/l	2/16/2017 14:05:34	
I1826-03D	S	Phenolics-	P	-0.0072	mg/l	2/16/2017 14:05:35	
I1826-03S	S	Phenolics-	P	0.8822	mg/l	2/16/2017 14:05:36	
I1826-03SD	S	Phenolics-	P	0.8865	mg/l	2/16/2017 14:05:37	
I1850-05	S	Phenolics-	P	-0.0005	mg/l	2/16/2017 14:05:38	
CCV2	S	Phenolics-	P	0.9785	mg/l	2/16/2017 14:05:39	
CCB2	S	Phenolics-	P	-0.004	mg/l	2/16/2017 14:09:26	

LB 85853

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Ak

2/16/2017 13:37

Test Phenolics-


Accepted 2/16/2017 13:37

Factor 9.196

Bias 0.006

Coeff. of det. 0.999988

Errors

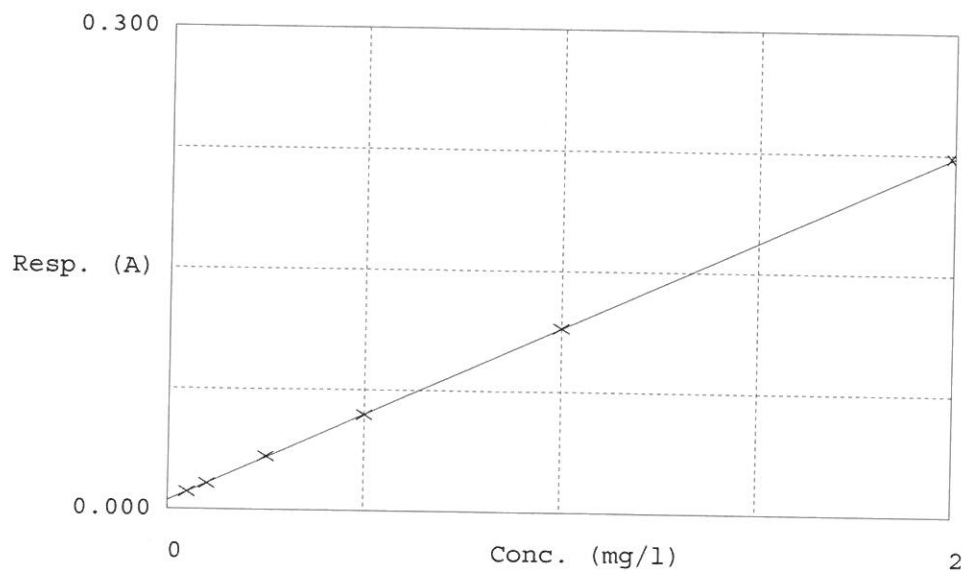

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.011	0.0497	0.0500	
2	Phenol-2	0.016	0.0978	0.1000	
3	Phenol-2	0.033	0.2541	0.2500	
4	Phenol-2	0.060	0.4972	0.5000	
5	Phenol-2	0.114	1.0018	1.0000	
6	Phenol-2	0.223	1.9994	2.0000	