

LB85964

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

2/22/2017 15:12

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	92.788	0.0	0.098	
ICB1	-0.189	0.0	0.005	
CCV1	238.743	0.0	0.244	
CCB1	-0.138	0.0	0.005	
PB97111BL	-0.025	0.0	0.006	
I1929-02	-0.497	0.0	0.005	
I1929-02DUP	0.196	0.0	0.006	
I1935-02	-0.162	0.0	0.005	
I1936-03	-0.100	0.0	0.006	
I1936-04	-0.363	0.0	0.005	
CCV2	239.024	0.0	0.244	
CCB2	-0.100	0.0	0.006	

N	12
Mean	47.431
SD	93.2952
CV%	196.70

LB 88964

Aquakem v. 7.2AQ1

Results from time period:

AK

Wed Feb 22 15:09:10 2017

Wed Feb 22 15:11:58 2017

Sample Id	Sam/Ctr/c	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.726	µg/l	2/22/2017 13:22:59	
5.OPPBCN	A	Reactive CN	P	4.5903	µg/l	2/22/2017 13:23:00	
10PPBCN	A	Reactive CN	P	9.4901	µg/l	2/22/2017 13:23:01	
50PPBCN	A	Reactive CN	P	49.7808	µg/l	2/22/2017 13:23:02	
100PPBCN	A	Reactive CN	P	101.4533	µg/l	2/22/2017 13:23:03	
250PPBCN	A	Reactive CN	P	251.3318	µg/l	2/22/2017 13:23:04	
500PPBCN	A	Reactive CN	P	499.0796	µg/l	2/22/2017 13:23:05	
ICV1	S	Reactive CN	P	92.7878	µg/l	2/22/2017 15:09:10	
ICB1	S	Reactive CN	P	-0.1894	µg/l	2/22/2017 15:09:11	
CCV1	S	Reactive CN	P	238.7425	µg/l	2/22/2017 15:09:12	
CCB1	S	Reactive CN	P	-0.1382	µg/l	2/22/2017 15:09:13	
PB97111BL	S	Reactive CN	P	-0.0248	µg/l	2/22/2017 15:09:14	
I1929-02	S	Reactive CN	P	-0.4968	µg/l	2/22/2017 15:09:15	
I1929-02DUP	S	Reactive CN	P	0.1962	µg/l	2/22/2017 15:09:16	
I1935-02	S	Reactive CN	P	-0.1624	µg/l	2/22/2017 15:09:17	
I1936-03	S	Reactive CN	P	-0.1004	µg/l	2/22/2017 15:09:18	
I1936-04	S	Reactive CN	P	-0.3634	µg/l	2/22/2017 15:09:19	
CCV2	S	Reactive CN	P	239.0241	µg/l	2/22/2017 15:09:20	
CCB2	S	Reactive CN	P	-0.0995	µg/l	2/22/2017 15:11:58	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

2/22/2017 13:25


Test Total CN

Accepted 2/22/2017 13:25

Factor 1001
Bias 0.006

Coeff. of det. 0.999972

Errors

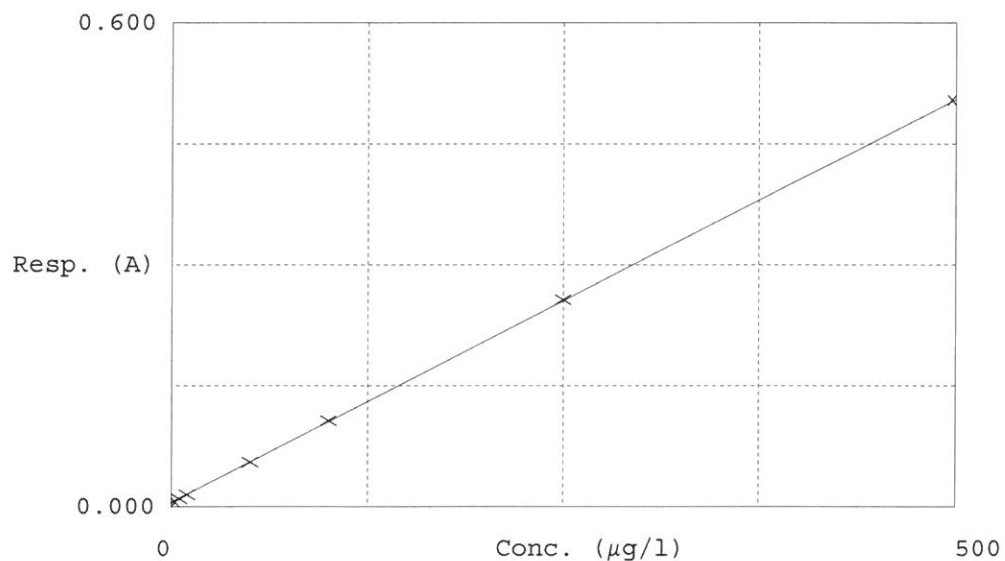

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.005	-0.7260	0.0000	
2	5.0PPBCN	0.010	4.5903	5.0000	
3	10PPBCN	0.015	9.4901	10.0000	
4	50PPBCN	0.055	49.7808	50.0000	
5	100PPBCN	0.107	101.4533	100.0000	
6	250PPBCN	0.257	251.3318	250.0000	
7	500PPBCN	0.504	499.0796	500.0000	