

CB86085

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

2/28/2017 15:36

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.861	0.0	0.088	
ICB1	-0.392	0.0	0.006	
CCV1	243.998	0.0	0.218	
CCB1	0.067	0.0	0.006	
PB97241BL	-0.238	0.0	0.006	
I2011-02	-0.925	0.0	0.005	
I2011-02DUP	-2.030	0.0	0.005	
PB97242BL	-0.444	0.0	0.006	
I2014-01	-0.884	0.0	0.006	
I2014-01DUP	-0.605	0.0	0.006	
CCV2	246.732	0.0	0.220	
CCB2	-0.171	0.0	0.006	

N	12
Mean	48.248
SD	95.9615
CV%	198.89

LB86085

Aquakem v. 7.2AQ1

Results from time period:

AK

Tue Feb 28 15:27:01 2017

Tue Feb 28 15:29:49 2017

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	CI P	0.2687	µg/l	2/28/2017 12:11:28	
5.OPPBCN	A	Reactive	CI P	3.9082	µg/l	2/28/2017 12:11:29	
10PPBCN	A	Reactive	CI P	9.6723	µg/l	2/28/2017 12:11:30	
50PPBCN	A	Reactive	CI P	49.1672	µg/l	2/28/2017 12:11:31	
100PPBCN	A	Reactive	CI P	100.6739	µg/l	2/28/2017 12:11:32	
250PPBCN	A	Reactive	CI P	252.6873	µg/l	2/28/2017 12:11:33	
500PPBCN	A	Reactive	CI P	498.6223	µg/l	2/28/2017 12:11:34	
ICV1	S	Reactive	CI P	93.8613	µg/l	2/28/2017 15:27:01	
ICB1	S	Reactive	CI P	-0.3921	µg/l	2/28/2017 15:27:02	
CCV1	S	Reactive	CI P	243.9984	µg/l	2/28/2017 15:27:03	
CCB1	S	Reactive	CI P	0.0673	µg/l	2/28/2017 15:27:04	
PB97241BL	S	Reactive	CI P	-0.2381	µg/l	2/28/2017 15:27:05	
I2011-02	S	Reactive	CI P	-0.9252	µg/l	2/28/2017 15:27:06	
I2011-02DUP	S	Reactive	CI P	-2.03	µg/l	2/28/2017 15:27:07	
PB97242BL	S	Reactive	CI P	-0.4441	µg/l	2/28/2017 15:27:08	
I2014-01	S	Reactive	CI P	-0.8835	µg/l	2/28/2017 15:27:09	
I2014-01DUP	S	Reactive	CI P	-0.6045	µg/l	2/28/2017 15:27:10	
CCV2	S	Reactive	CI P	246.7324	µg/l	2/28/2017 15:27:11	
CCB2	S	Reactive	CI P	-0.1712	µg/l	2/28/2017 15:29:49	

===== CB 86085 =====
Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : OK

2/28/2017 15:28


Test Total CN

Accepted 2/28/2017 12:19

Factor 1154
Bias 0.006

Coeff. of det. 0.999943

Errors

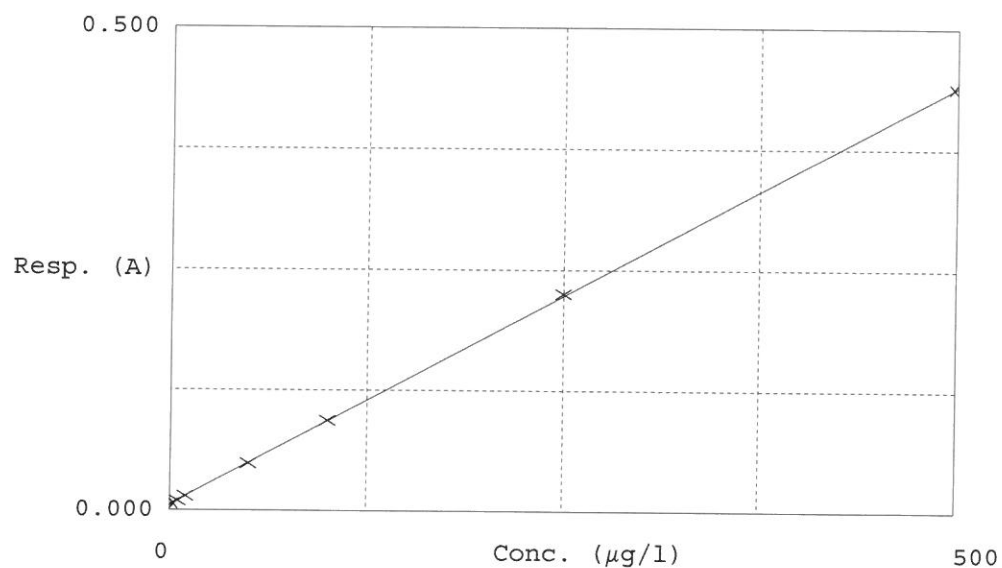

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.007	0.2687	0.0000	
2	5.0PPBCN	0.010	3.9082	5.0000	
3	10PPBCN	0.015	9.6723	10.0000	
4	50PPBCN	0.049	49.1672	50.0000	
5	100PPBCN	0.094	100.6739	100.0000	
6	250PPBCN	0.225	252.6873	250.0000	
7	500PPBCN	0.438	498.6223	500.0000	