

CB86179

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

3/6/2017 13:01

Test: Total CN

Sample Id	Result ^{MSIL}	Dil. 1 +	Response	Errors
ICV1	92.547	0.0	0.092	
ICB1	0.530	0.0	0.005	
CCV1	240.538	0.0	0.231	
CCB1	0.438	0.0	0.005	
PB97349BL	0.125	0.0	0.004	
I2100-02	0.086	0.0	0.004	
I2100-02DUP	0.008	0.0	0.004	
PB97350BL	0.500	0.0	0.005	
I2103-01	-0.079	0.0	0.004	
I2103-01DUP	0.215	0.0	0.004	
CCV2	243.496	0.0	0.234	
CCB2	-0.137	0.0	0.004	

N	12
Mean	48.189
SD	94.3150
CV%	195.72

CB 86179

Aquakem v. 7.2AQ1

Results from time period:

Mon Mar 06 12:38:06 2017

Mon Mar 06 12:40:54 2017

AK

Sample Id	Sam/Ctr/c	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.1829	µg/l	3/6/2017 10:49:07	
5.OPPBCN	A	Reactive CN	P	4.633	µg/l	3/6/2017 10:49:08	
10PPBCN	A	Reactive CN	P	9.763	µg/l	3/6/2017 10:49:09	
50PPBCN	A	Reactive CN	P	49.337	µg/l	3/6/2017 10:49:10	
100PPBCN	A	Reactive CN	P	100.3791	µg/l	3/6/2017 10:49:11	
250PPBCN	A	Reactive CN	P	252.1439	µg/l	3/6/2017 10:49:12	
500PPBCN	A	Reactive CN	P	498.9269	µg/l	3/6/2017 10:49:13	
ICV1	S	Reactive CN	P	92.5472	µg/l	3/6/2017 12:38:06	
ICB1	S	Reactive CN	P	0.5297	µg/l	3/6/2017 12:38:07	
CCV1	S	Reactive CN	P	240.5375	µg/l	3/6/2017 12:38:08	
CCB1	S	Reactive CN	P	0.4384	µg/l	3/6/2017 12:38:09	
PB97349BL	S	Reactive CN	P	0.1252	µg/l	3/6/2017 12:38:10	
I2100-02	S	Reactive CN	P	0.086	µg/l	3/6/2017 12:38:11	
I2100-02DUP	S	Reactive CN	P	0.0077	µg/l	3/6/2017 12:38:12	
PB97350BL	S	Reactive CN	P	0.5	µg/l	3/6/2017 12:38:13	
I2103-01	S	Reactive CN	P	-0.0788	µg/l	3/6/2017 12:38:14	
I2103-01DUP	S	Reactive CN	P	0.2146	µg/l	3/6/2017 12:38:15	
CCV2	S	Reactive CN	P	243.4963	µg/l	3/6/2017 12:38:16	
CCB2	S	Reactive CN	P	-0.1367	µg/l	3/6/2017 12:40:54	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AK

3/6/2017 12:15


Test Total CN

Accepted 3/6/2017 11:04

Factor 1058
 Bias 0.004

Coeff. of det. 0.999968

Errors

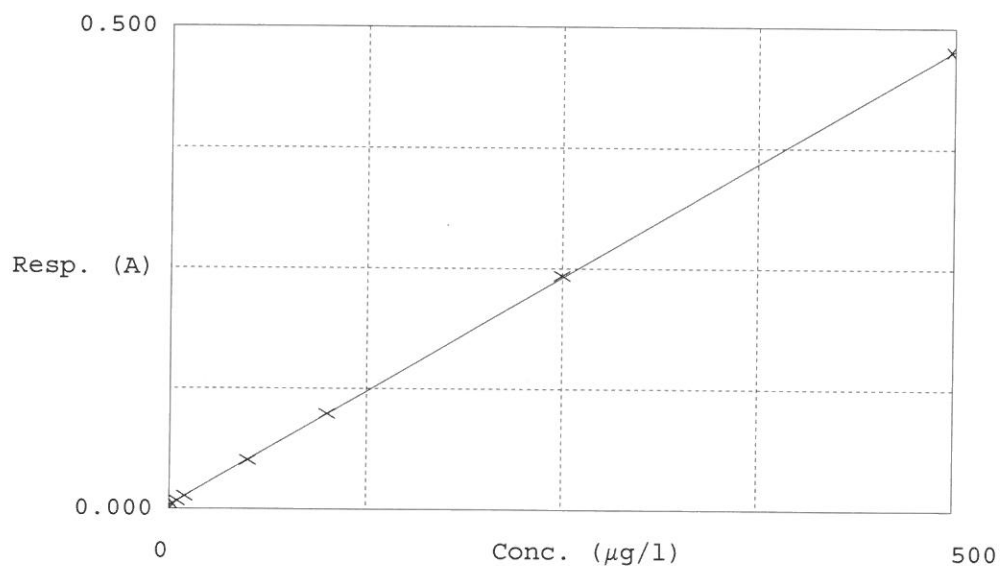

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.1829	0.0000	
2	5.0PPBCN	0.009	4.6330	5.0000	
3	10PPBCN	0.013	9.7630	10.0000	
4	50PPBCN	0.051	49.3370	50.0000	
5	100PPBCN	0.099	100.3791	100.0000	
6	250PPBCN	0.242	252.1439	250.0000	
7	500PPBCN	0.476	498.9269	500.0000	