

LB86538

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

3/24/2017 13:57

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.116	0.0	0.084	
ICB1	0.537	0.0	0.004	
CCV1	238.794	0.0	0.210	
CCB1	0.491	0.0	0.004	
PB97772BL	0.789	0.0	0.005	
PB97772BS	98.262	0.0	0.089	
MIDPB97772	243.835	0.0	0.214	
I2273-02	1.135	0.0	0.005	
I2273-02DUP	0.758	0.0	0.005	
I2273-02MS	33.949	0.0	0.033	
I2273-02MSD	34.241	0.0	0.033	
CCV2	259.469	0.0	0.228	
CCB2	-0.054	0.0	0.004	

N	13
Mean	77.332
SD	102.7587
CV%	132.88

LB 86538

Aquakem v. 7.2AQ1

Results from time period:

AK

Fri Mar 24 12:26:42 2017

Fri Mar 24 13:39:19 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.0238	µg/l	3/24/2017 12:26:42	
5.OPPBCN	A	Total CN	P	4.577	µg/l	3/24/2017 12:26:43	
10PPBCN	A	Total CN	P	9.7536	µg/l	3/24/2017 12:26:44	
50PPBCN	A	Total CN	P	49.3143	µg/l	3/24/2017 12:26:45	
100PPBCN	A	Total CN	P	100.0214	µg/l	3/24/2017 12:26:46	
250PPBCN	A	Total CN	P	252.4727	µg/l	3/24/2017 12:26:47	
500PPBCN	A	Total CN	P	498.8371	µg/l	3/24/2017 12:26:48	
ICV1	S	Total CN	P	93.1159	µg/l	3/24/2017 13:15:36	
ICB1	S	Total CN	P	0.5368	µg/l	3/24/2017 13:15:37	
CCV1	S	Total CN	P	238.7941	µg/l	3/24/2017 13:15:38	
CCB1	S	Total CN	P	0.4914	µg/l	3/24/2017 13:15:39	
PB97772BL	S	Total CN	P	0.7892	µg/l	3/24/2017 13:15:40	
PB97772BS	S	Total CN	P	98.2621	µg/l	3/24/2017 13:15:41	
MIDPB97772	S	Total CN	P	243.835	µg/l	3/24/2017 13:15:42	
I2273-02	S	Total CN	P	1.1351	µg/l	3/24/2017 13:15:43	
I2273-02DUP	S	Total CN	P	0.7577	µg/l	3/24/2017 13:15:44	
I2273-02MS	S	Total CN	P	33.9489	µg/l	3/24/2017 13:15:45	
I2273-02MSD	S	Total CN	P	34.2406	µg/l	3/24/2017 13:39:17	
CCV2	S	Total CN	P	259.4688	µg/l	3/24/2017 13:39:18	
CCB2	S	Total CN	P	-0.0539	µg/l	3/24/2017 13:39:19	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AK

3/24/2017 12:36


Test Total CN

Accepted 3/24/2017 12:36

Factor 1159
 Bias 0.004

Coeff. of det. 0.999960

Errors

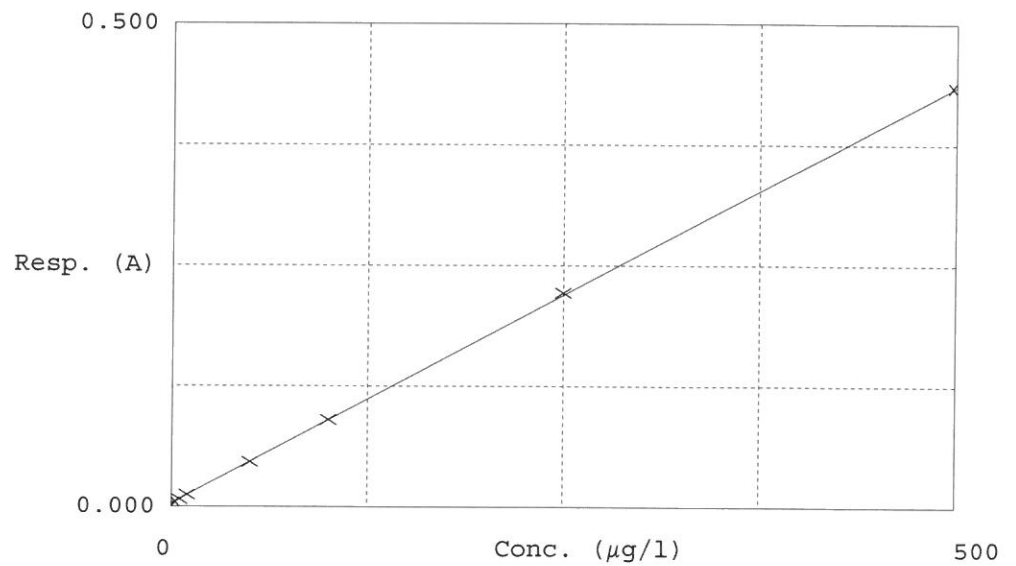

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.0238	0.0000	
2	5.0PPBCN	0.008	4.5770	5.0000	
3	10PPBCN	0.012	9.7536	10.0000	
4	50PPBCN	0.046	49.3143	50.0000	
5	100PPBCN	0.090	100.0214	100.0000	
6	250PPBCN	0.222	252.4727	250.0000	
7	500PPBCN	0.434	498.8371	500.0000	