


Clear table

M9056
IC-4
AK 4/11/17

ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-04-07_	4/7/17 12:39
STD2	0.1090	0.2230	0.2470	0.6030	0.1930	0.1430	1.0980	2017-04-07_	4/7/17 13:10
STD3	0.4220	0.6310	0.6230	2.1060	0.5310	0.9610	3.1720	2017-04-07_	4/7/17 13:41
STD4	0.7830	1.1820	1.1680	3.9910	0.9810	2.0450	5.9110	2017-04-07_	4/7/17 14:11
STD5	1.9860	2.9060	2.8830	9.7400	2.3970	5.2530	14.4960	2017-04-07_	4/7/17 14:42
STD6	3.9710	5.8890	5.9310	19.8560	4.9340	9.8050	29.5160	2017-04-07_	4/7/17 15:13
STD7	5.0290	7.6200	7.5980	25.2040	6.3390	12.5440	38.0570	2017-04-07_	4/7/17 15:44
ICV	2.0740	2.9350	2.9600	10.1290	2.4430	5.3080	14.7210	2017-04-07_	4/7/17 18:26
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-04-07_	4/7/17 18:57
CCV	2.0830	2.9410	2.9210	9.9210	2.4310	5.3050	14.6630	2017-04-07_	4/7/17 21:32
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-04-07_	4/7/17 22:02
LB86774BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-04-07_	4/7/17 22:33
LB86774BSW	2.1410	2.9880	3.0020	10.0660	2.4840	5.3560	14.8110	2017-04-07_	4/7/17 23:04
I2296-05	0.0800	0.1120	0.1350	0.3280	0.1090	-0.0790	0.5830	2017-04-07_	4/7/17 23:35
I2296-06	0.2370	0.3680	0.3690	1.2440	0.3240	0.4510	1.8840	2017-04-08_	4/8/17 0:06
CCV	2.0960	2.9350	2.9290	9.9590	2.4230	5.3100	14.6020	2017-04-08_	4/8/17 0:37
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-04-08_	4/8/17 1:08

CALIBRATION OF COMPONENT F-

Method: ANIONS 04-07-17.mtw
 Equation: $Q = 0.875956 \cdot A + 1.25922$
 RSD: 1.266 %
 Correlation coefficient: 0.999935

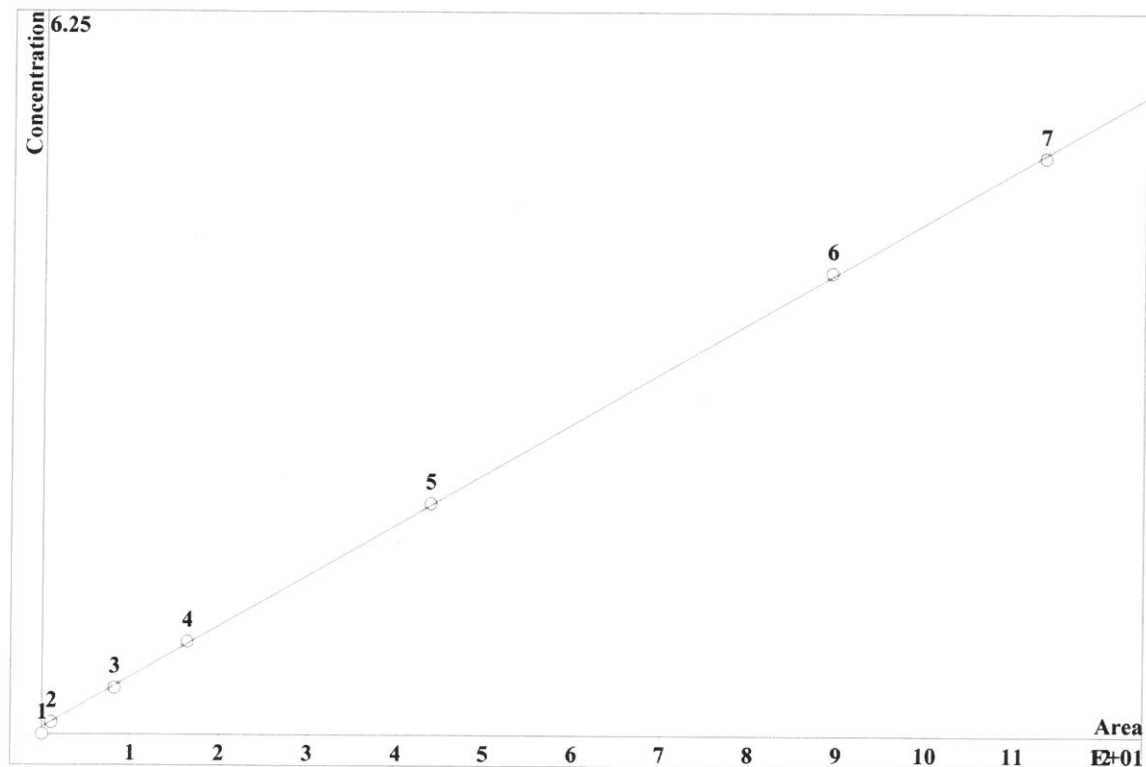


K3 = 0 K2 = 0 K1 = 0.875956 K0 = 1.25922

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.06084	1.049	0.1	20	5.749			Yes
3	0.3908	8.193	0.4	20	5.749			Yes
4	0.8008	16.45	0.8	20	5.749			Yes
5	2.068	43.9	2	20	5.749			Yes
6	4.37	89.24	4	20	5.749			Yes
7	5.631	113.4	5	20	5.749			Yes

CALIBRATION OF COMPONENT CL-

Method: ANIONS 04-07-17.mtw
 Equation: $Q = 1.29946 \cdot A + 1.58339$
 RSD: 3.329 %
 Correlation coefficient: 0.999548

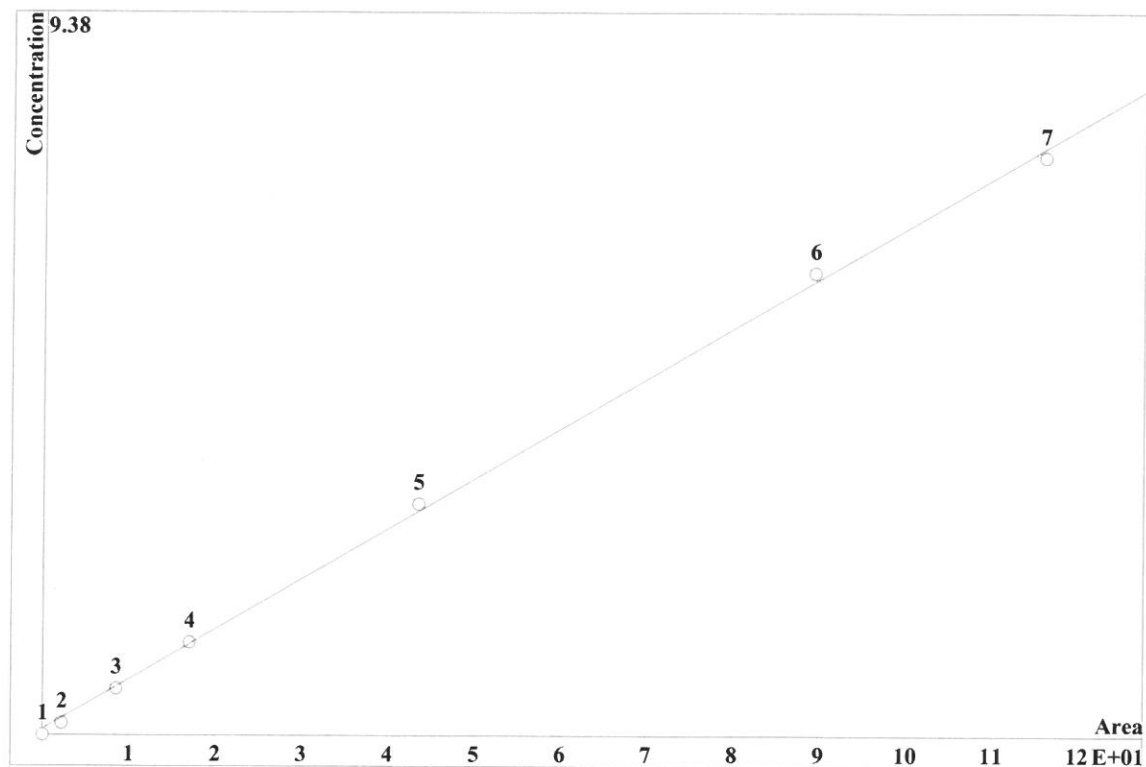


K3 = 0 K2 = 0 K1 = 1.29946 K0 = 1.58339

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.1143	2.209	0.15	20	8.479	Yes	
3	0.4449	8.488	0.6	20	8.479	Yes	
4	0.8894	16.97	1.2	20	8.479	Yes	
5	2.312	43.51	3	20	8.479	Yes	
6	4.783	89.42	6	20	8.479	Yes	
7	6.203	116.1	7.5	20	8.479	Yes	

CALIBRATION OF COMPONENT NO2

Method: ANIONS 04-07-17.mtw
 Equation: $Q = 0.556971 \cdot A + 2.34401$
 RSD: 3.220 %
 Correlation coefficient: 0.999577

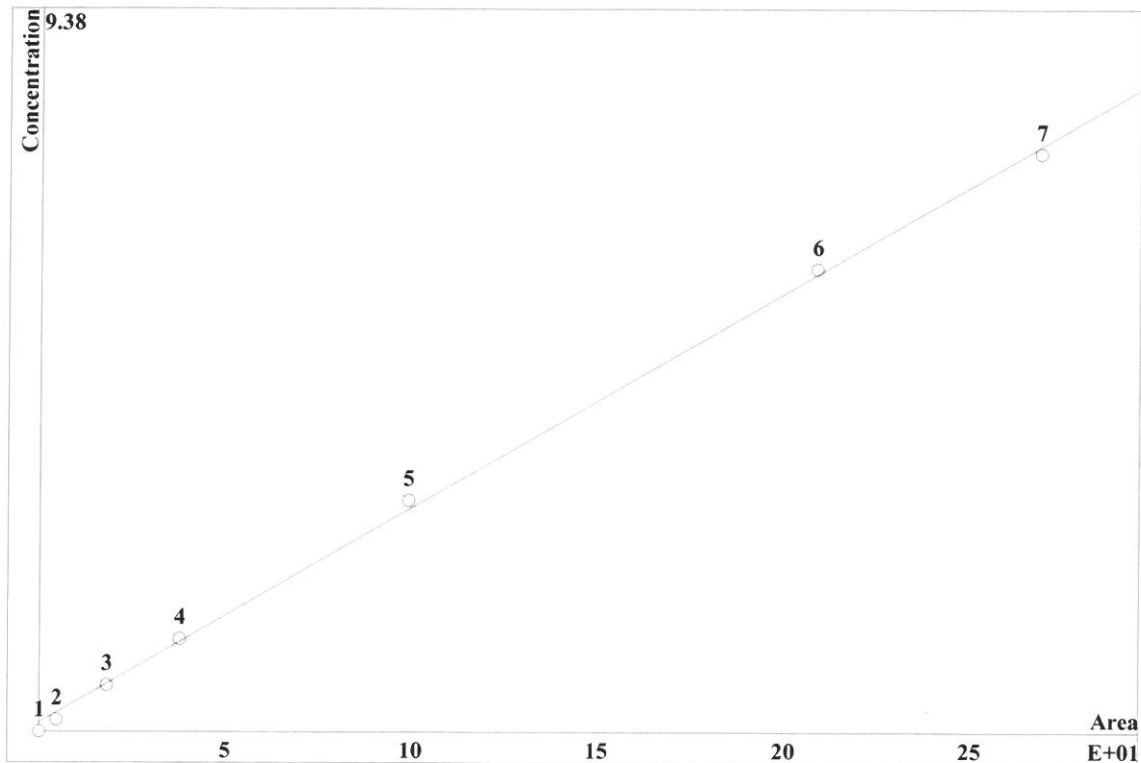


K3 = 0 K2 = 0 K1 = 0.556971 K0 = 2.34401
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.2022	4.662	0.15	20	10.05			Yes
3	0.8747	18.17	0.6	20	10.05			Yes
4	1.782	37.73	1.2	20	10.05			Yes
5	4.729	99.31	3	20	10.05			Yes
6	9.869	208.8	6	20	10.05			Yes
7	12.66	268.6	7.5	20	10.05			Yes

±□; \$

CALIBRATION OF COMPONENT BR-

Method: ANIONS 04-07-17.mtw
 Equation: $Q = 2.94908 \cdot A - 8.05712$
 RSD: 1.901 %
 Correlation coefficient: 0.999853

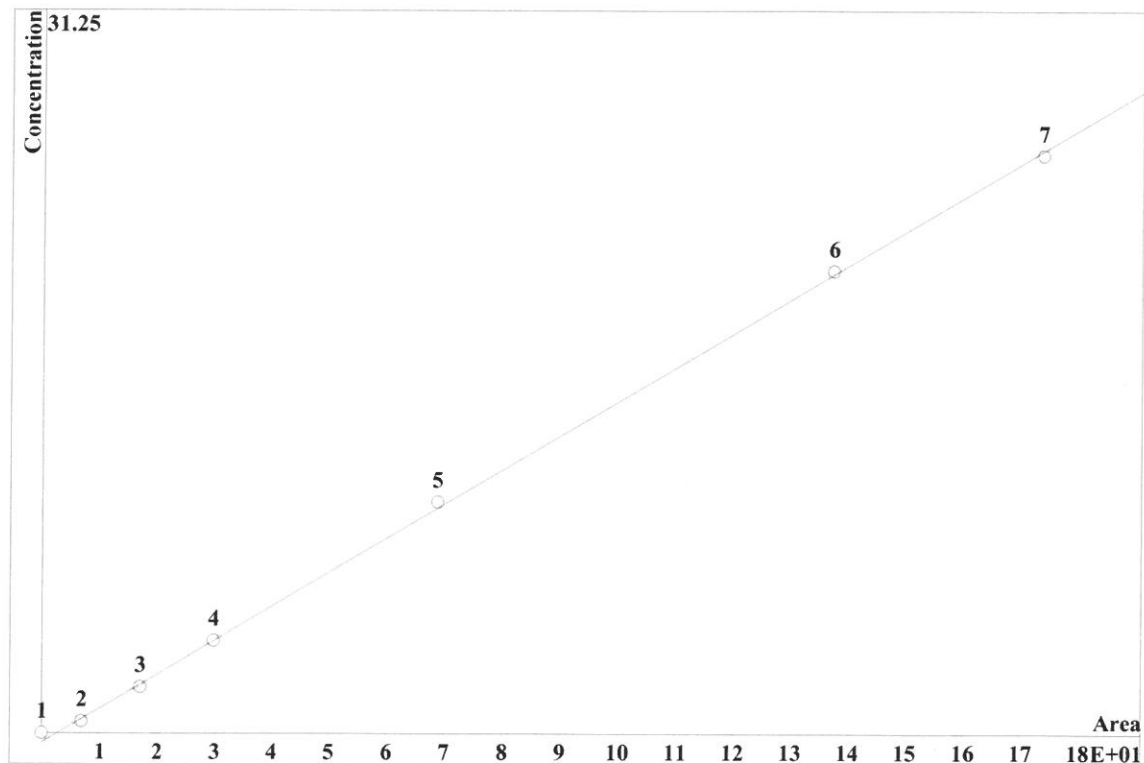


K3 = 0 K2 = 0 K1 = 2.94908 K0 = -8.05712

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.1655	6.82	0.5	20	12.84	Yes	
3	0.5217	17.02	2	20	12.84	Yes	
4	0.9785	29.8	4	20	12.84	Yes	
5	2.273	68.79	10	20	12.84	Yes	
6	4.2	137.4	20	20	12.84	Yes	
7	4.966	173.7	25	20	12.84	Yes	

CALIBRATION OF COMPONENT NO3

Method: ANIONS 04-07-17.mtw
 Equation: $Q = 0.51206 \cdot A + 1.95153$
 RSD: 3.317 %
 Correlation coefficient: 0.999551

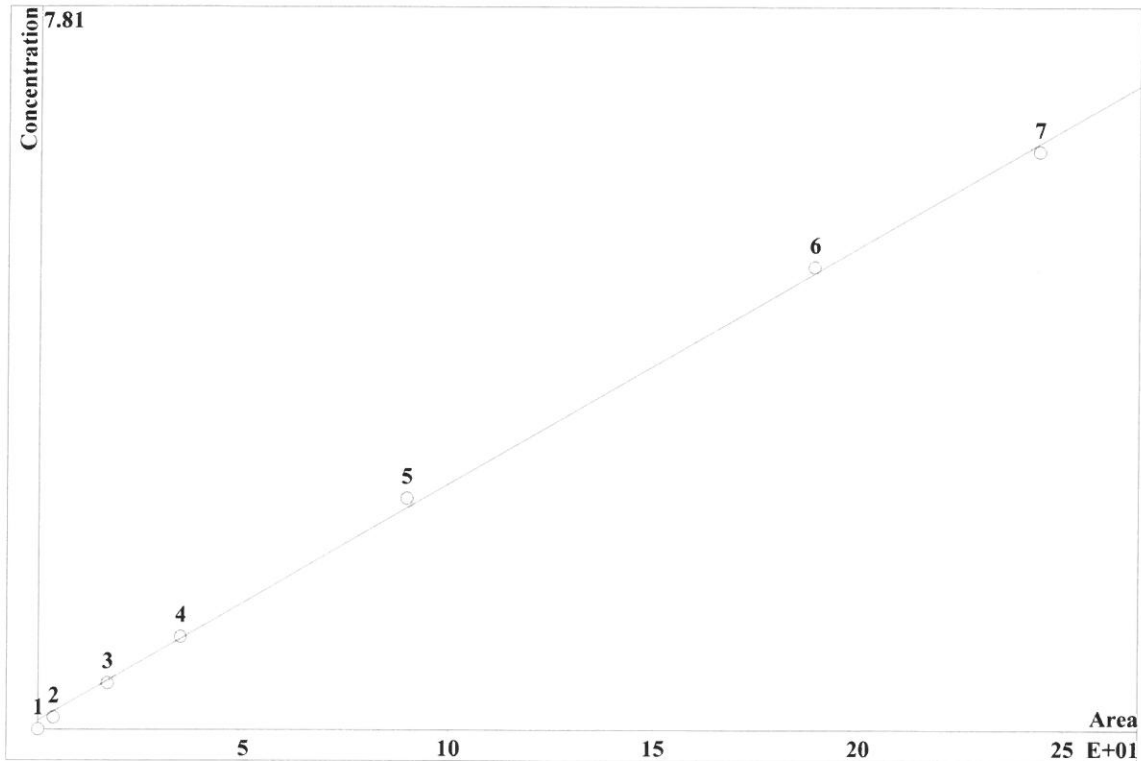


K3 = 0 K2 = 0 K1 = 0.51206 K0 = 1.95153
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.1408	3.739	0.125	20	14.38			Yes
3	0.6337	16.94	0.5	20	14.38			Yes
4	1.292	34.49	1	20	14.38			Yes
5	3.386	89.82	2.5	20	14.38			Yes
6	7.088	188.9	5	20	14.38			Yes
7	9.083	243.8	6.25	20	14.38			Yes

CALIBRATION OF COMPONENT HPO4

Method: ANIONS 04-07-17.mtw
 Equation: $Q = 1.33502 \cdot A - 2.19947$
 RSD: 3.364 %
 Correlation coefficient: 0.999538

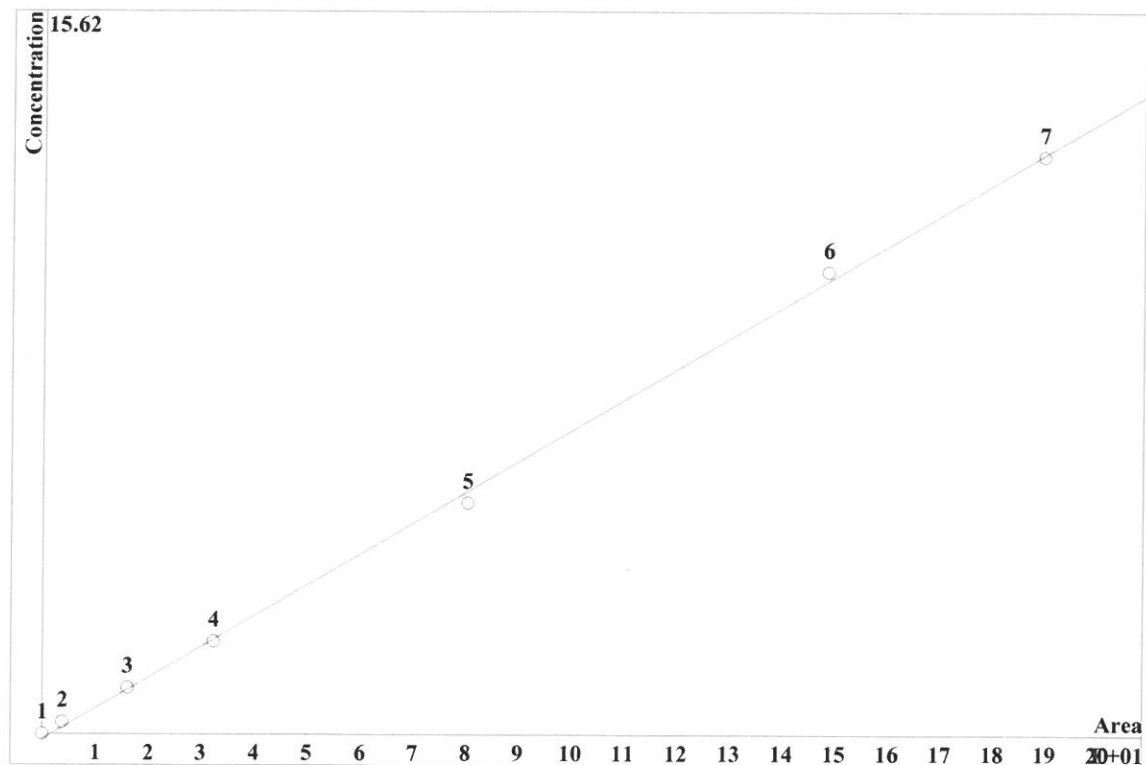


K3 = 0 K2 = 0 K1 = 1.33502 K0 = -2.19947

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0		0	0	0		No
2	0.07035	3.786	0.25	20	20.62	Yes	
3	0.2575	16.05	1	20	20.62	Yes	
4	0.5772	32.28	2	20	20.62	Yes	
5	1.474	80.34	5	20	20.62	Yes	
6	2.741	148.5	10	20	20.62	Yes	
7	3.605	189.6	12.5	20	20.62	Yes	

CALIBRATION OF COMPONENT SO4

Method: ANIONS 04-07-17.mtw
 Equation: $Q = 1.6994 \cdot A + 7.96215$
 RSD: 3.182 %
 Correlation coefficient: 0.999587

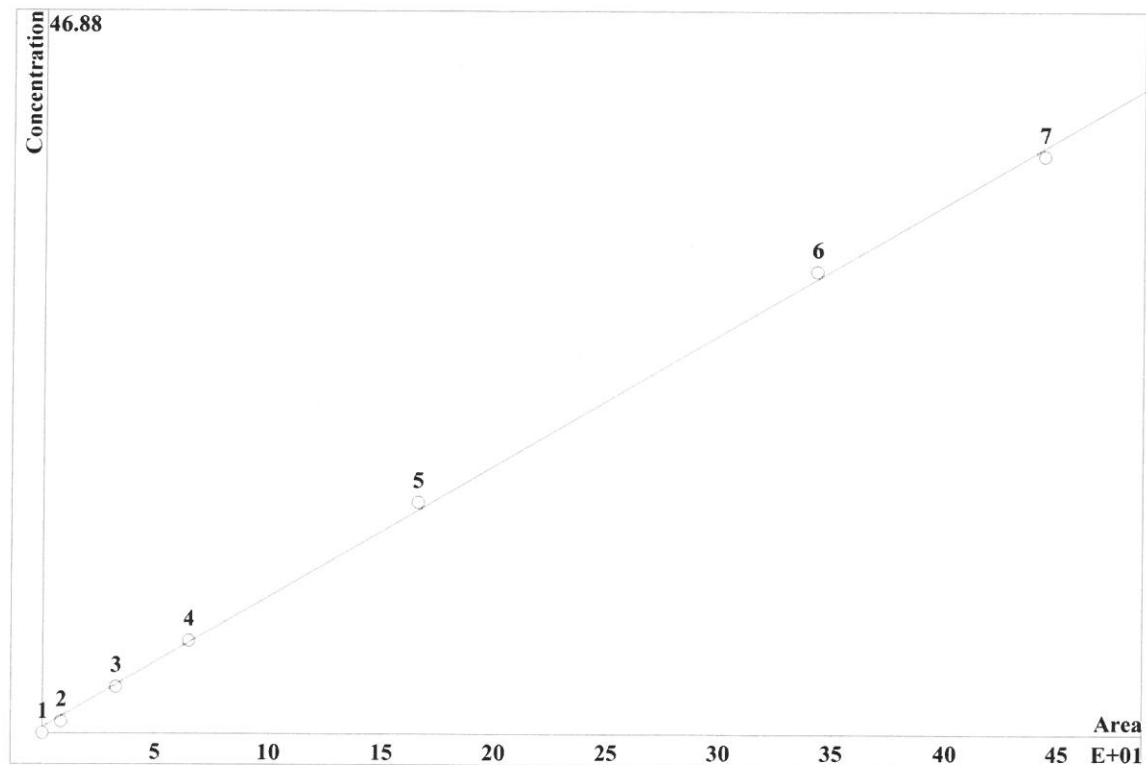

K3 = 0 K2 = 0 K1 = 1.6994 K0 = 7.96215

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.1614	8.241	0.75	20	23.34			Yes
3	0.6174	32.65	3	20	23.34			Yes
4	1.234	64.88	6	20	23.34			Yes
5	3.199	165.9	15	20	23.34			Yes
6	6.644	342.7	30	20	23.34			Yes
7	8.659	443.2	37.5	20	23.34			Yes

Report date: 4/10/2017 9:57:51 AM
Printed by: wet


Ident: STD1
Analysis from: 4/7/2017 12:39:12 PM
File: _2017-04-07_

Last save: 4/7/2017 4:14:34 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57034

Last save: 4/7/2017 12:29:24 PM

SAMPLE:
: AP/AK
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

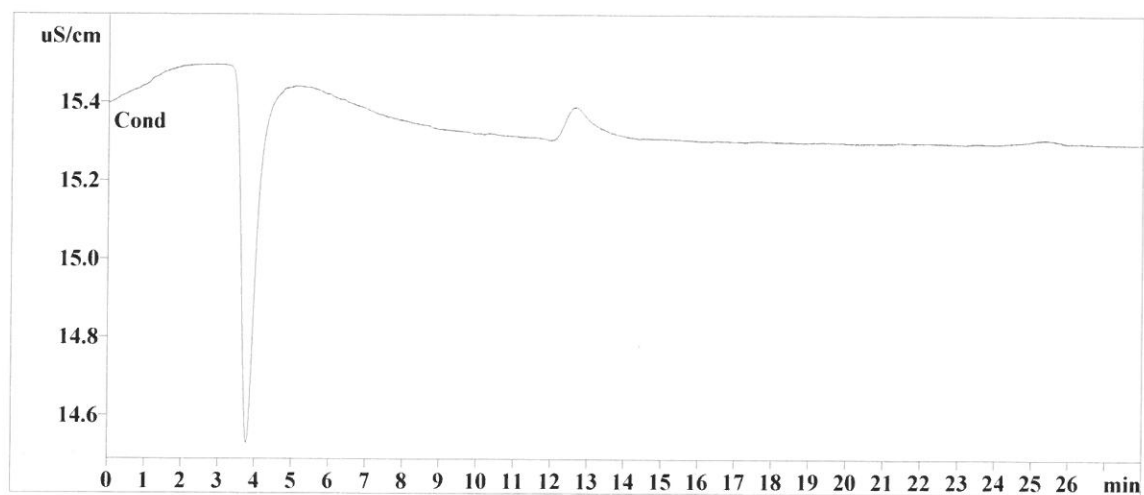

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/10/2017 9:57:56 AM
Printed by: wet


Ident: STD2
Analysis from: 4/7/2017 1:10:07 PM
File: _2017-04-07_

Last save: 4/7/2017 4:14:34 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57035

Last save: 4/7/2017 12:29:24 PM

SAMPLE:
: AP/AK
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

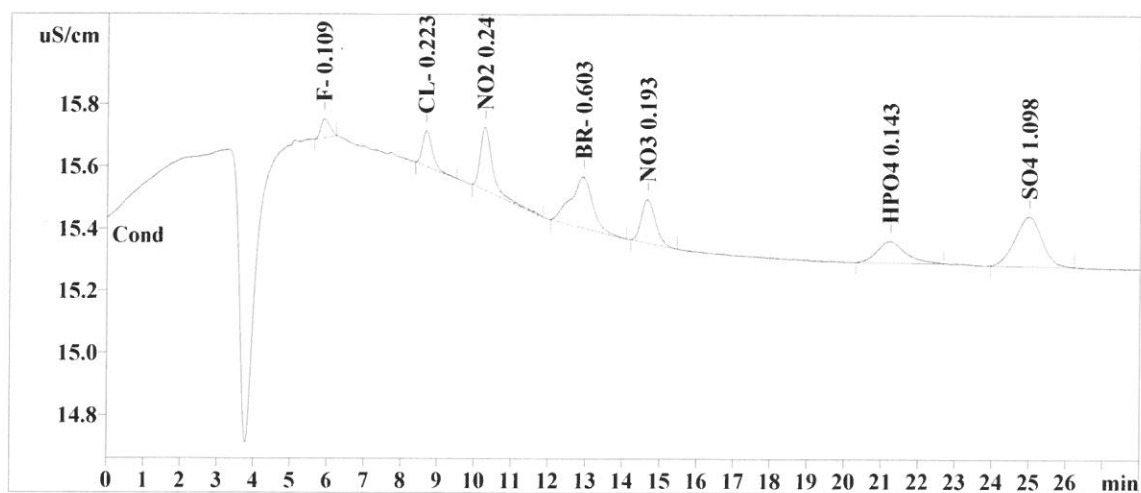

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.90	0.284	0.06	6.59	1.049	3.44	0.
2	8.68	0.286	0.11	12.43	2.209	7.24	0.
3	10.28	0.318	0.20	22.02	4.662	15.28	0.
4	12.93	0.604	0.16	18.00	6.820	22.36	0.
5	14.65	0.411	0.14	15.27	3.739	12.26	0.
6	21.24	0.794	0.07	7.60	3.786	12.41	0.
7	25.00	0.793	0.16	17.54	8.241	27.01	0.
7	28.00	0.499	0.91	99.46	30.506	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/10/2017 9:58:02 AM
Printed by: wet


Ident: STD3
Analysis from: 4/7/2017 1:41:01 PM
File: _2017-04-07_

Last save: 4/7/2017 4:14:34 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57036

Last save: 4/7/2017 12:29:24 PM

SAMPLE:
: AP/AK
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

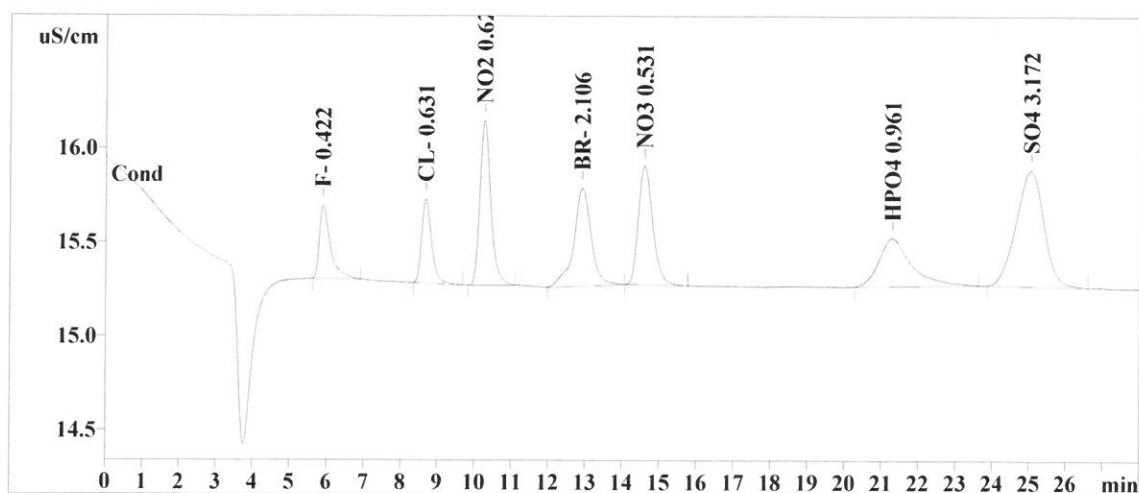

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.294	0.39	10.43	8.193	6.97	0.
2	8.67	0.283	0.44	11.89	8.488	7.22	0.
3	10.25	0.311	0.87	23.38	18.167	15.46	0.
4	12.91	0.448	0.52	13.92	17.016	14.48	0.
5	14.58	0.406	0.63	16.92	16.944	14.42	0.
6	21.28	0.855	0.26	6.87	16.048	13.66	0.
7	25.04	0.813	0.62	16.49	32.645	27.78	0.
7	28.00	0.487	3.74	99.90	117.502	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/10/2017 9:58:07 AM
Printed by: wet


Ident: STD4
Analysis from: 4/7/2017 2:11:56 PM
File: _2017-04-07_

Last save: 4/7/2017 4:14:34 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57037

Last save: 4/7/2017 12:29:24 PM

SAMPLE:
: AP/AK
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

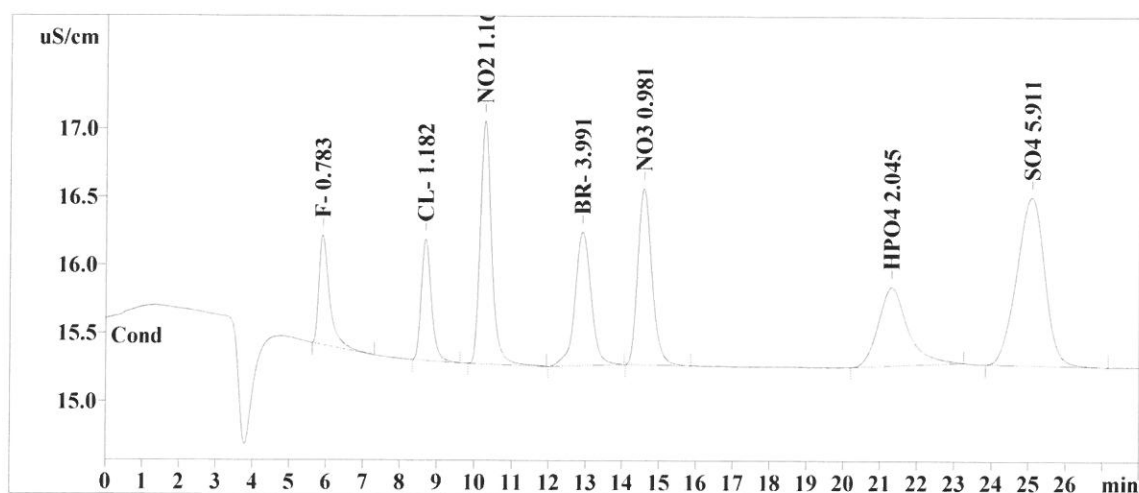

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.290	0.80	10.60	16.451	7.07	0.
2	8.68	0.286	0.89	11.77	16.971	7.30	0.
3	10.26	0.310	1.78	23.59	37.729	16.22	0.
4	12.90	0.444	0.98	12.95	29.798	12.81	0.
5	14.57	0.405	1.29	17.10	34.492	14.83	0.
6	21.30	0.797	0.58	7.63	32.280	13.88	0.
7	25.07	0.812	1.23	16.33	64.880	27.89	0.
7	28.00	0.478	7.55	99.97	232.601	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/10/2017 9:58:12 AM
Printed by: wet


Ident: STD5
Analysis from: 4/7/2017 2:42:50 PM
File: _2017-04-07_

Last save: 4/7/2017 4:14:34 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57038

Last save: 4/7/2017 12:29:24 PM

SAMPLE:
: AP/AK
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

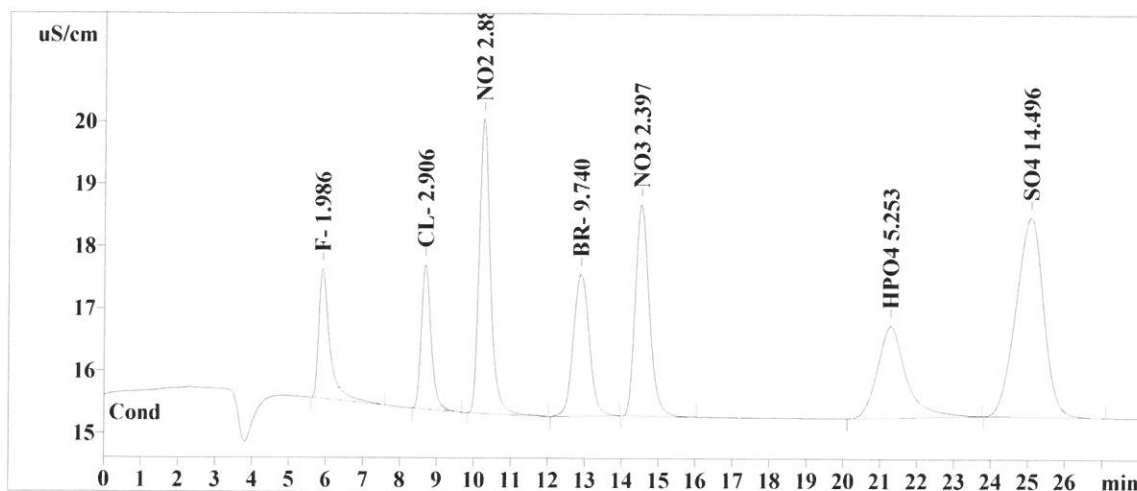

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.90	0.289	2.07	10.64	43.899	7.42	0.
2	8.68	0.280	2.31	11.89	43.508	7.35	0.
3	10.25	0.308	4.73	24.33	99.311	16.79	0.
4	12.89	0.465	2.27	11.69	68.786	11.63	0.
5	14.52	0.402	3.39	17.41	89.816	15.18	0.
6	21.28	0.765	1.47	7.58	80.340	13.58	0.
7	25.07	0.801	3.20	16.45	165.915	28.05	0.
7	28.00	0.473	19.44	99.99	591.574	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/10/2017 9:58:17 AM
Printed by: wet


Ident: STD6
Analysis from: 4/7/2017 3:13:45 PM
File: _2017-04-07_

Last save: 4/7/2017 4:14:34 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57039

Last save: 4/7/2017 12:29:24 PM

SAMPLE:
: AP/AK
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

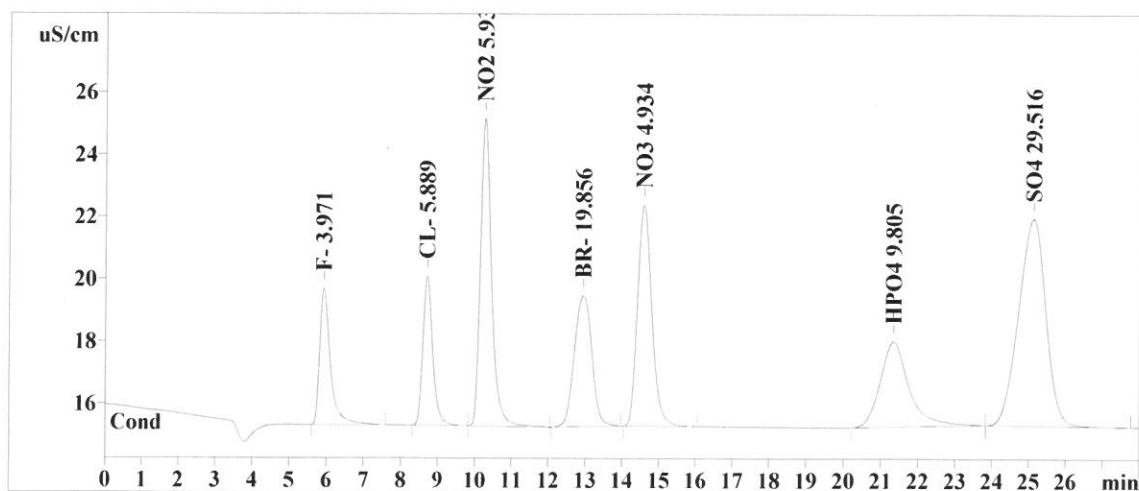

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.92	0.286	4.37	11.01	89.235	7.41	0.
2	8.70	0.277	4.78	12.05	89.424	7.42	0.
3	10.26	0.310	9.87	24.86	208.751	17.32	0.
4	12.94	0.514	4.20	10.58	137.392	11.40	0.
5	14.58	0.404	7.09	17.86	188.888	15.68	0.
6	21.34	0.766	2.74	6.90	148.535	12.33	0.
7	25.11	0.801	6.64	16.74	342.686	28.44	0.
7	28.00	0.480	39.69	100.00	1204.911	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/10/2017 9:58:24 AM
 Printed by: wet


Ident: STD7
 Analysis from: 4/7/2017 3:44:40 PM
 File: _2017-04-07_

Last save: 4/7/2017 4:23:46 PM

Method: ANIONS 04-07-17.mtw
 Run operator: wet
 Analysis number: 57040

Last save: 4/7/2017 12:29:24 PM

SAMPLE:
 : AK/AP
 Vial number: 8
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

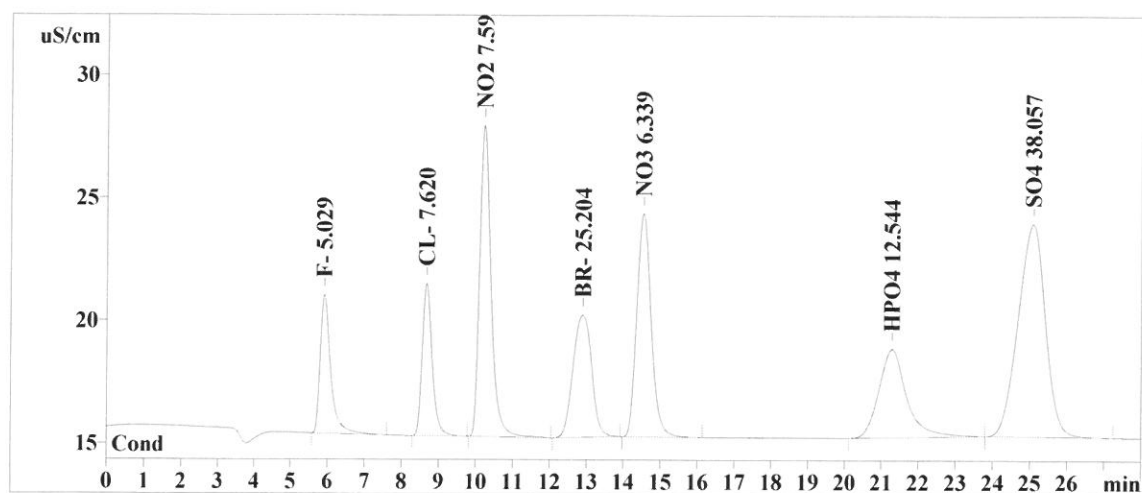

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.90	0.286	5.63	11.08	113.384	7.32	0.
2	8.66	0.278	6.20	12.21	116.054	7.50	0.
3	10.21	0.312	12.66	24.92	268.642	17.35	0.
4	12.89	0.554	4.97	9.77	173.659	11.22	0.
5	14.52	0.408	9.08	17.88	243.770	15.74	0.
6	21.28	0.748	3.60	7.09	189.562	12.24	0.
7	25.07	0.794	8.66	17.04	443.201	28.63	0.
7	28.00	0.483	50.81	100.00	1548.271	100.00	0.

This report has been created by IC Net
 METROHM LTD

Report date: 4/10/2017 9:58:31 AM
Printed by: wet


Ident: ICV
Analysis from: 4/7/2017 6:26:39 PM
File: _2017-04-07_

Last save: 4/7/2017 6:54:28 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57045

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

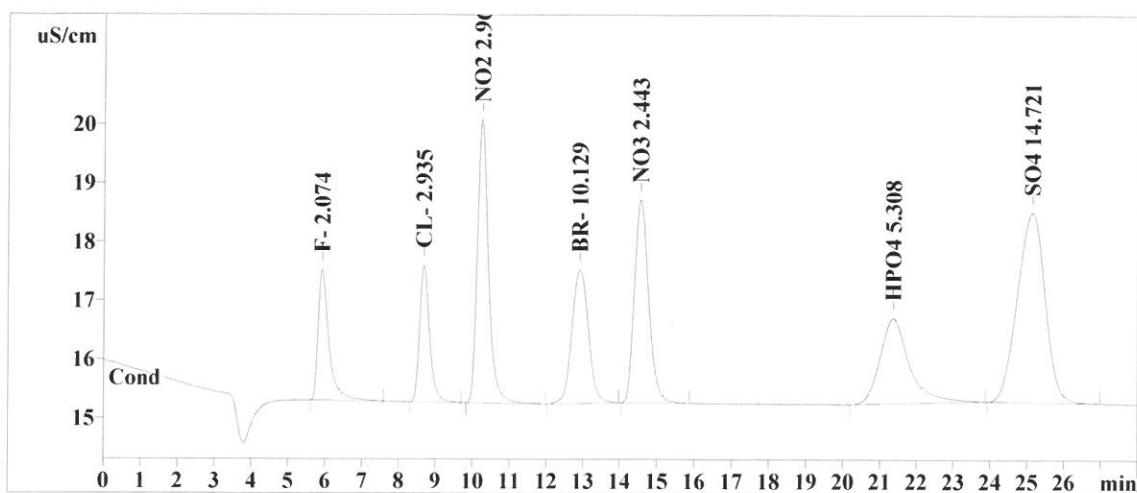

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.91	0.289	2.22	11.22	45.920	7.59	0.
2	8.67	0.281	2.32	11.76	43.957	7.27	0.
3	10.24	0.310	4.82	24.40	102.079	16.88	0.
4	12.91	0.485	2.27	11.49	71.427	11.81	0.
5	14.54	0.404	3.45	17.47	91.603	15.15	0.
6	21.35	0.791	1.45	7.32	81.164	13.42	0.
7	25.13	0.818	3.23	16.32	168.568	27.88	0.
7	28.00	0.483	19.77	99.98	604.720	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/10/2017 10:01:31 AM
Printed by: wet


Ident: ICB
Analysis from: 4/7/2017 6:57:33 PM
File: _2017-04-07_

Last save: 4/10/2017 9:59:06 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57046

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

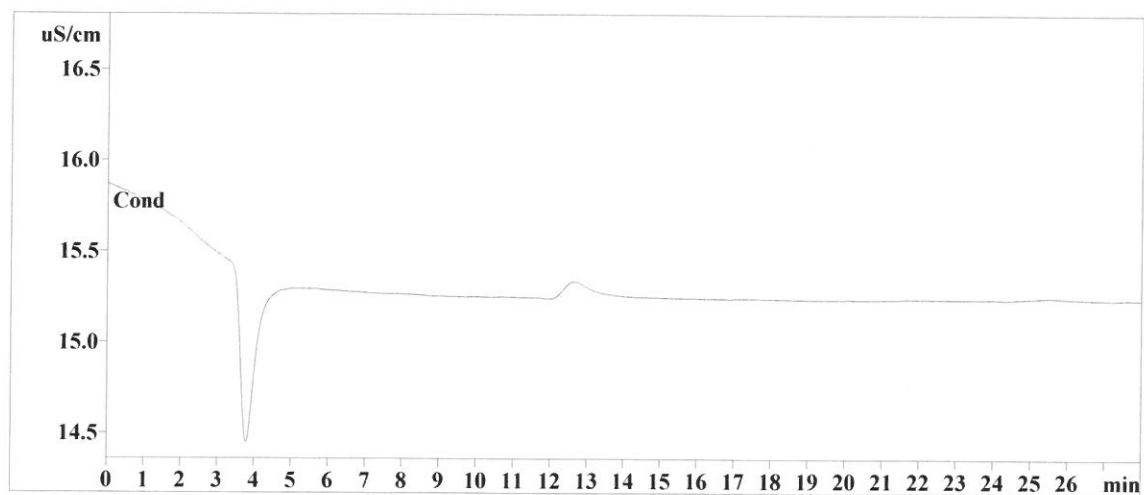

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:01:46 PM
Printed by: wet


Ident: CCV
Analysis from: 4/7/2017 9:32:05 PM
File: _2017-04-07_

Last save: 4/7/2017 9:59:54 PM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57051

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

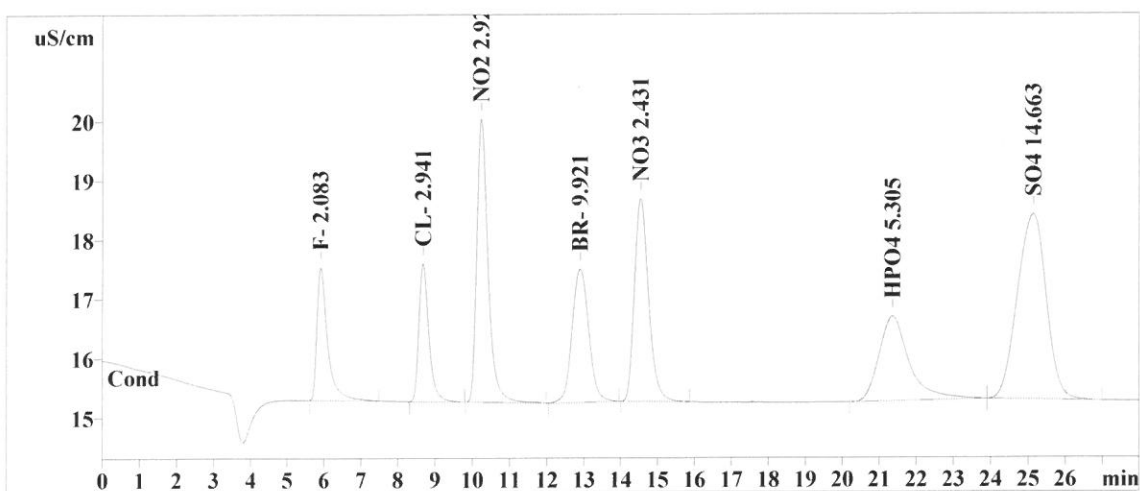

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.91	0.288	2.23	11.42	46.130	7.68	0.
2	8.68	0.280	2.33	11.90	44.051	7.33	0.
3	10.24	0.308	4.77	24.42	100.683	16.75	0.
4	12.90	0.480	2.24	11.48	70.011	11.65	0.
5	14.53	0.405	3.42	17.49	91.120	15.16	0.
6	21.36	0.805	1.43	7.31	81.128	13.50	0.
7	25.13	0.846	3.12	15.98	167.880	27.93	0.
7	28.00	0.487	19.55	99.99	601.003	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:01:57 PM
Printed by: wet


Ident: CCB
Analysis from: 4/7/2017 10:02:59 PM
File: _2017-04-07_

Last save: 4/10/2017 9:59:08 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57052

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

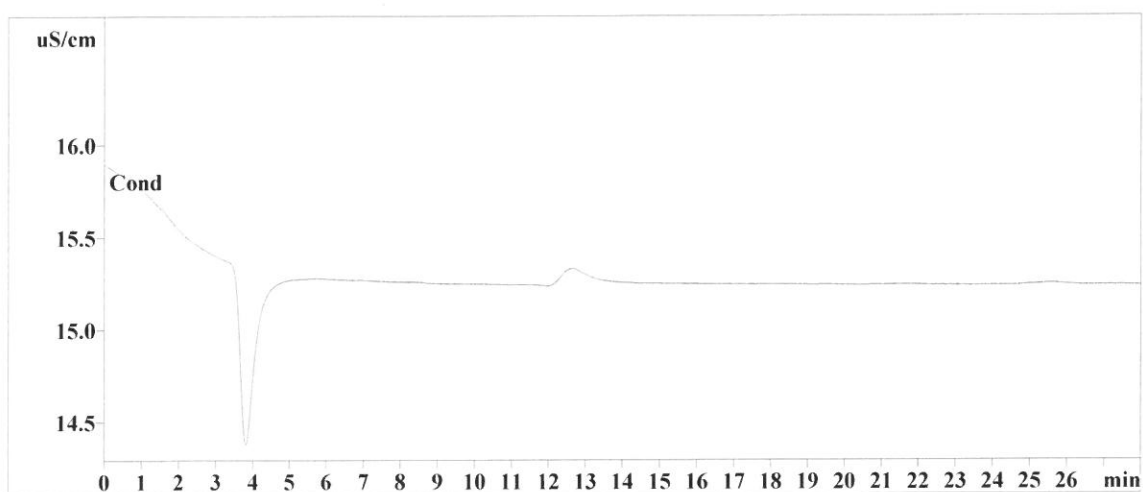

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:02:05 PM
Printed by: wet


Ident: LB86774BLW
Analysis from: 4/7/2017 10:33:54 PM
File: _2017-04-07_

Last save: 4/10/2017 9:59:08 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57053

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

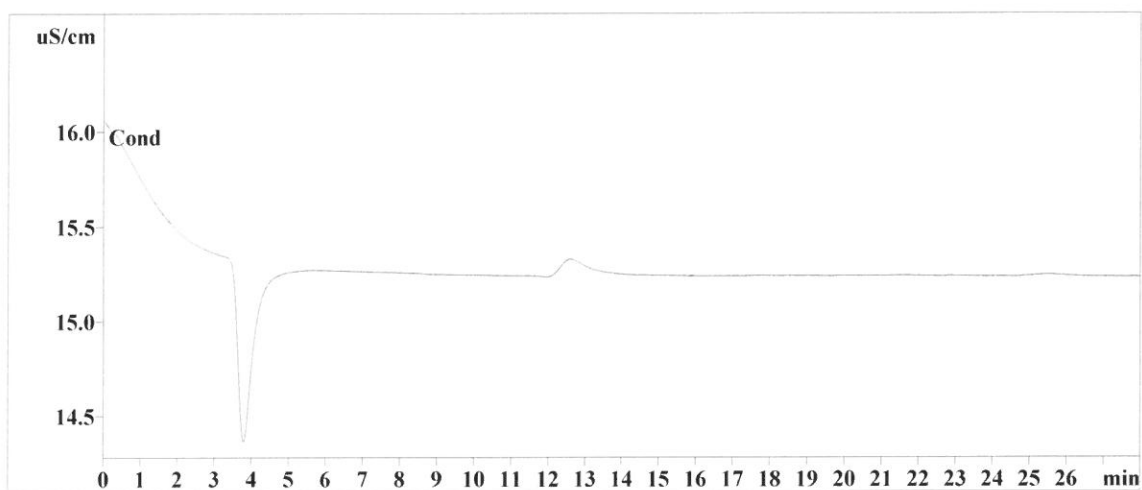

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:02:11 PM
Printed by: wet


Ident: LB86774BSW
Analysis from: 4/7/2017 11:04:48 PM
File: _2017-04-07_

Last save: 4/10/2017 9:32:24 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57054

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

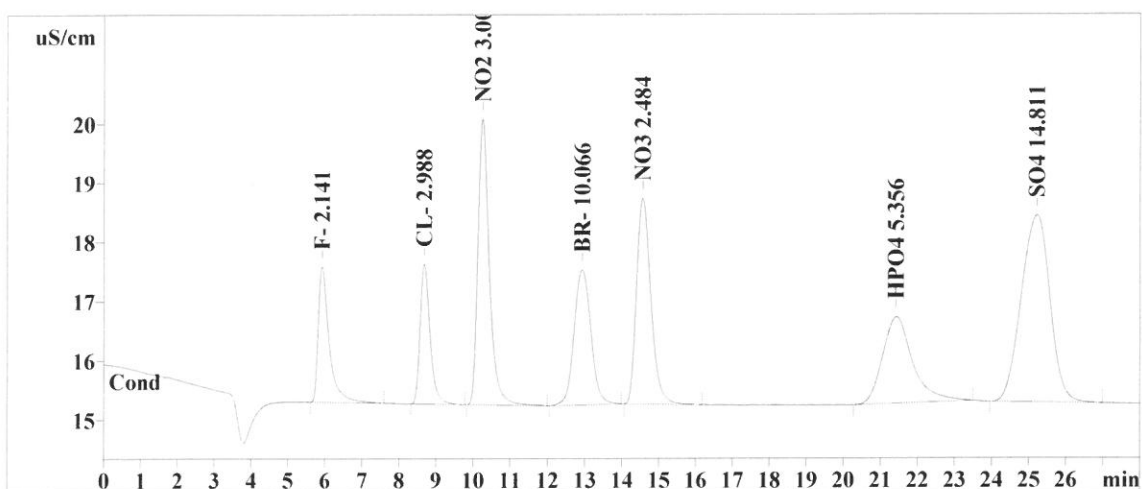

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.92	0.290	2.28	11.49	47.454	7.76	0.
2	8.68	0.281	2.36	11.90	44.770	7.32	0.
3	10.25	0.314	4.83	24.35	103.592	16.94	0.
4	12.93	0.481	2.27	11.46	70.996	11.61	0.
5	14.55	0.407	3.47	17.52	93.189	15.24	0.
6	21.43	0.814	1.46	7.35	81.883	13.39	0.
7	25.22	0.848	3.15	15.92	169.619	27.74	0.
7	28.00	0.491	19.82	99.99	611.504	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:02:17 PM
Printed by: wet

Ident: I2296-05
Analysis from: 4/7/2017 11:35:42 PM
File: _2017-04-07_


Last save: 4/10/2017 10:06:32 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57055

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

*Before
peaks not
by software
4/13/17*

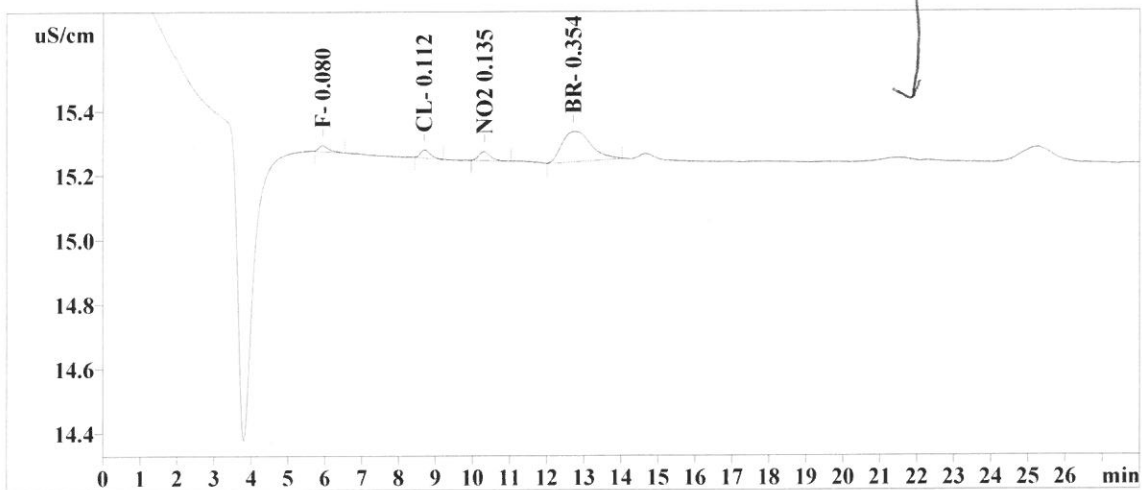

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.94	0.279	0.02	11.41	0.397	5.96	0.
2	8.69	0.293	0.03	15.04	0.505	7.58	0.
3	10.32	0.324	0.03	16.49	0.626	9.40	0.
4	12.72	0.846	0.09	55.16	5.130	77.06	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	28.00	0.249	0.17	98.10	6.656	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:22:04 PM
Printed by: wet

Ident: I2296-05
Analysis from: 4/7/2017 11:35:42 PM
File: _2017-04-07_

Last save: 4/13/2017 4:21:36 PM


Manual peaks!

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57055

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

After
nl
4/13/17

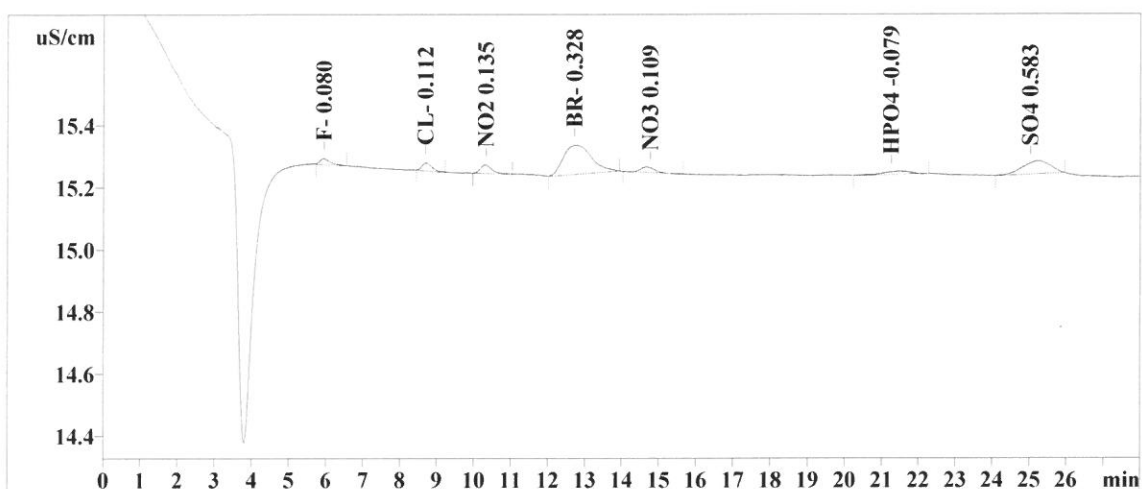

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.94	0.279	0.02	8.61	0.397	4.15	0.
2	8.69	0.293	0.03	11.35	0.505	5.28	0.
3	10.32	0.324	0.03	12.44	0.626	6.54	0.
4	12.71	0.838	0.09	41.15	4.955	51.80	0.
5	14.76	0.438	0.02	6.73	0.439	4.58	0.
6	21.24	0.881	0.01	3.57	0.464	4.85	0.
7	25.02	0.945	0.04	15.65	2.181	22.81	0.
7	28.00	0.571	0.23	99.49	9.565	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:22:13 PM
Printed by: wet


Ident: I2296-06
Analysis from: 4/8/2017 12:06:37 AM
File: _2017-04-08_

Last save: 4/8/2017 12:34:26 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57056

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

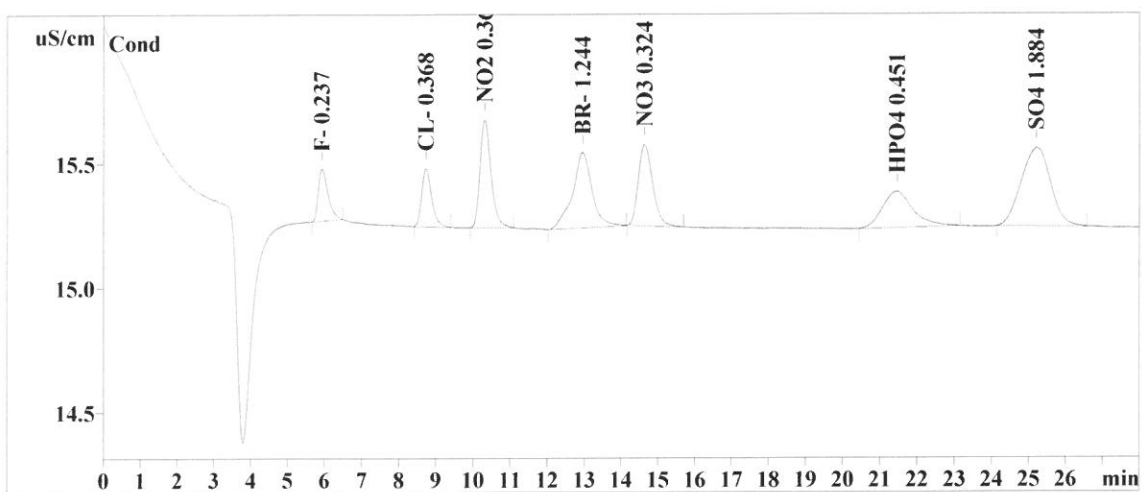

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.93	0.286	0.21	10.66	3.970	6.27	0.
2	8.73	0.288	0.23	11.82	4.449	7.02	0.
3	10.31	0.314	0.43	21.93	9.025	14.25	0.
4	12.95	0.501	0.30	15.36	11.167	17.63	0.
5	14.63	0.411	0.33	16.62	8.847	13.97	0.
6	21.46	0.847	0.15	7.41	8.401	13.26	0.
7	25.22	0.876	0.31	15.97	17.484	27.60	0.
7	28.00	0.503	1.97	99.77	63.342	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:22:18 PM
Printed by: wet


Ident: CCV
Analysis from: 4/8/2017 12:37:31 AM
File: _2017-04-08_

Last save: 4/8/2017 1:05:20 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57057

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

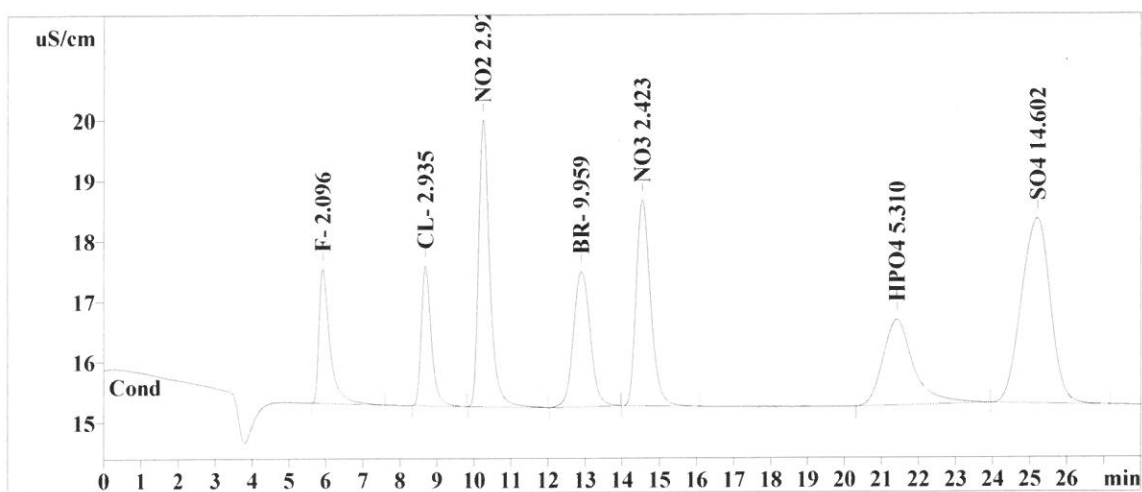

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.92	0.291	2.22	11.47	46.427	7.73	0.
2	8.68	0.282	2.31	11.91	43.957	7.32	0.
3	10.24	0.311	4.74	24.45	100.971	16.81	0.
4	12.90	0.484	2.24	11.52	70.271	11.70	0.
5	14.54	0.406	3.40	17.54	90.840	15.12	0.
6	21.41	0.818	1.42	7.30	81.200	13.51	0.
7	25.20	0.862	3.06	15.79	167.158	27.82	0.
7	28.00	0.493	19.39	99.98	600.825	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 4/13/2017 4:22:28 PM
Printed by: wet


Ident: CCB
Analysis from: 4/8/2017 1:08:25 AM
File: _2017-04-08_

Last save: 4/10/2017 9:59:08 AM

Method: ANIONS 04-07-17.mtw
Run operator: wet
Analysis number: 57058

Last save: 4/7/2017 4:23:50 PM

SAMPLE:
: AK/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

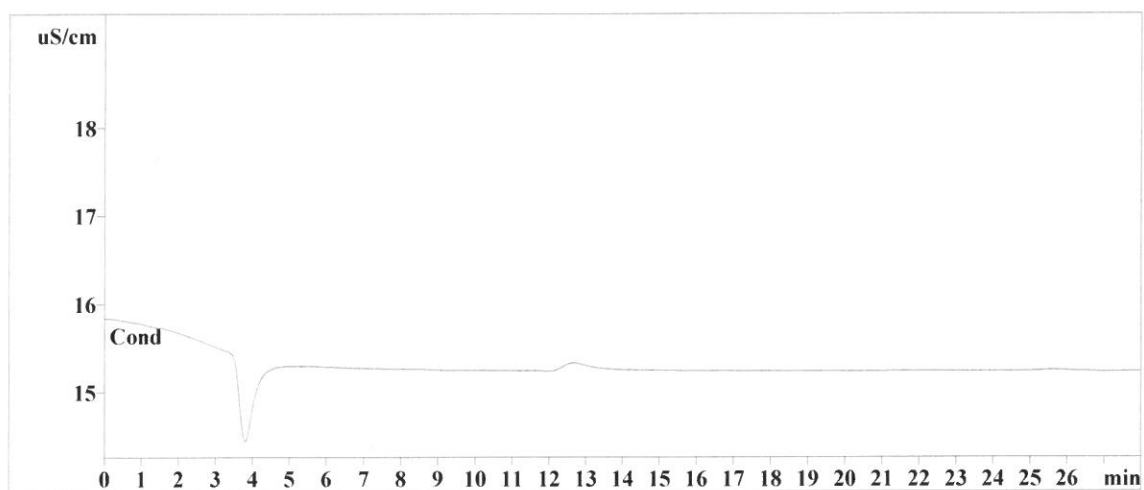

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD