

LB 87244

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

5/4/2017 11:55

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.033	0.0	0.112	
ICB1	0.004	0.0	0.002	
CCV1	1.046	0.0	0.113	
CCB1	0.001	0.0	0.002	
PB98679BL	0.004	0.0	0.002	
PB98679BS	1.040	0.0	0.113	
I2936-05	0.003	0.0	0.002	
I2936-05DUP	0.002	0.0	0.002	
I2936-05MS	0.888	0.0	0.096	
I2936-05MSD	0.884	0.0	0.096	
I2936-11	0.005	0.0	0.002	
I2936-17	0.003	0.0	0.002	
I2953-03	0.011	0.0	0.003	
CCV2	1.034	0.0	0.112	
CCB2	0.001	0.0	0.002	

N	15
Mean	0.397
SD	0.5012
CV%	126.16

Aquakem v. 7.2AQ1

Results from time period:

Thu May 04 11:50:57 2017

Thu May 04 11:55:25 2017

AK LB 87244

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0528	mg/l	5/4/2017 9:03:04	
0.1PPM	A	Phenolics-	P	0.1046	mg/l	5/4/2017 9:03:05	
0.25PPM	A	Phenolics-	P	0.2506	mg/l	5/4/2017 9:03:06	
0.50PPM	A	Phenolics-	P	0.4965	mg/l	5/4/2017 9:03:07	
1.0PPM	A	Phenolics-	P	0.9898	mg/l	5/4/2017 9:03:08	
2.0PPM	A	Phenolics-	P	2.0056	mg/l	5/4/2017 9:03:09	
ICV1	S	Phenolics-	P	1.0328	mg/l	5/4/2017 11:50:57	
ICB1	S	Phenolics-	P	0.0038	mg/l	5/4/2017 11:50:58	
CCV1	S	Phenolics-	P	1.0464	mg/l	5/4/2017 11:50:59	
CCB1	S	Phenolics-	P	0.0006	mg/l	5/4/2017 11:51:00	
PB98679BL	S	Phenolics-	P	0.0038	mg/l	5/4/2017 11:51:01	
PB98679BS	S	Phenolics-	P	1.0402	mg/l	5/4/2017 11:51:02	
I2936-05	S	Phenolics-	P	0.0029	mg/l	5/4/2017 11:51:03	
I2936-05DUP	S	Phenolics-	P	0.0016	mg/l	5/4/2017 11:51:04	
I2936-05MS	S	Phenolics-	P	0.8879	mg/l	5/4/2017 11:51:05	
I2936-05MSD	S	Phenolics-	P	0.8844	mg/l	5/4/2017 11:51:06	
I2936-11	S	Phenolics-	P	0.0047	mg/l	5/4/2017 11:51:07	
I2936-17	S	Phenolics-	P	0.0033	mg/l	5/4/2017 11:51:08	
I2953-03	S	Phenolics-	P	0.0115	mg/l	5/4/2017 11:55:23	
CCV2	S	Phenolics-	P	1.0345	mg/l	5/4/2017 11:55:24	
CCB2	S	Phenolics-	P	0.001	mg/l	5/4/2017 11:55:25	

LB87244

=====

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

5/4/2017 9:05

Test Phenolics-


Accepted 5/4/2017 9:04

Factor 9.368

Bias 0.002

Coeff. of det. 0.999937

Errors

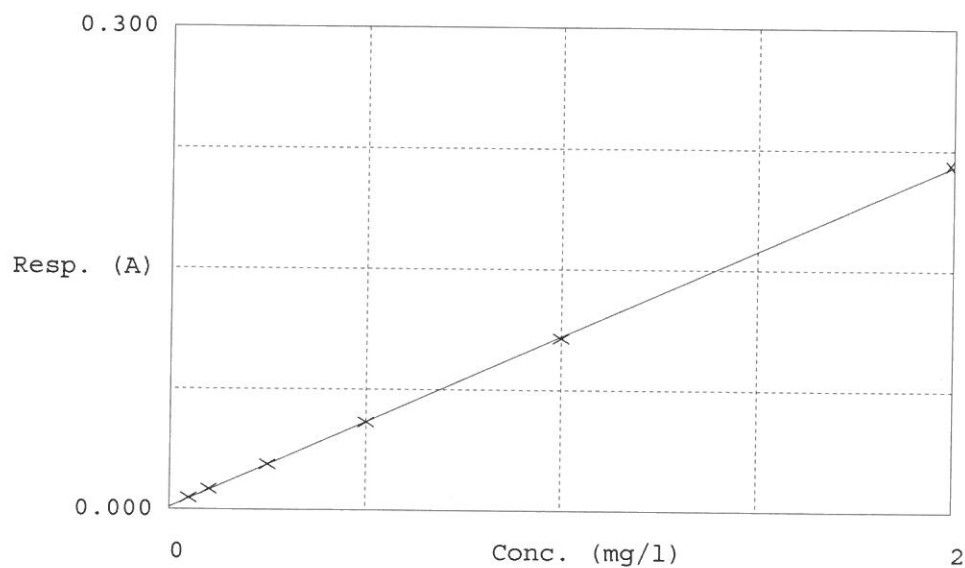

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.007	0.0528	0.0500	
2	Phenol-2	0.013	0.1046	0.1000	
3	Phenol-2	0.028	0.2506	0.2500	
4	Phenol-2	0.055	0.4965	0.5000	
5	Phenol-2	0.107	0.9898	1.0000	
6	Phenol-2	0.216	2.0056	2.0000	