

U881368

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

5/10/2017 14:26

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.934	0.0	0.106	
ICB1	-1.273	0.0	0.004	
CCV1	245.660	0.0	0.265	
CCB1	-1.355	0.0	0.004	
PB98852BL	-0.924	0.0	0.004	
PB98852BS	98.691	0.0	0.110	
MIDPB98852	250.802	0.0	0.270	
I3055-01	-0.684	0.0	0.005	
I3055-01DUP	-0.815	0.0	0.005	
I3055-01MS	27.986	0.0	0.035	
I3055-01MSD	28.129	0.0	0.035	
CCV2	253.014	0.0	0.272	
CCB2	-1.231	0.0	0.004	

N	13
Mean	76.380
SD	104.7858
CV%	137.19

CB 87368

Aquakem v. 7.2AQ1

AK

Results from time period:

Wed May 10 13:42:28 2017

Wed May 10 14:21:08 2017

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-1.2671	µg/l	5/10/2017 13:42:28	
5.OPPBCN	A	Total CN	P	3.6615	µg/l	5/10/2017 13:42:29	
10PPBCN	A	Total CN	P	8.5219	µg/l	5/10/2017 13:42:30	
50PPBCN	A	Total CN	P	50.2121	µg/l	5/10/2017 13:42:31	
100PPBCN	A	Total CN	P	101.3832	µg/l	5/10/2017 13:42:32	
250PPBCN	A	Total CN	P	255.4866	µg/l	5/10/2017 13:42:33	
500PPBCN	A	Total CN	P	497.0018	µg/l	5/10/2017 13:42:34	
ICV1	S	Total CN	P	94.9337	µg/l	5/10/2017 14:17:15	
ICB1	S	Total CN	P	-1.2734	µg/l	5/10/2017 14:17:16	
CCV1	S	Total CN	P	245.6602	µg/l	5/10/2017 14:17:17	
CCB1	S	Total CN	P	-1.3554	µg/l	5/10/2017 14:17:18	
PB98852BL	S	Total CN	P	-0.9239	µg/l	5/10/2017 14:17:19	
PB98852BS	S	Total CN	P	98.6908	µg/l	5/10/2017 14:17:20	
MIDPB98852	S	Total CN	P	250.8023	µg/l	5/10/2017 14:17:21	
I3055-01	S	Total CN	P	-0.684	µg/l	5/10/2017 14:17:22	
I3055-01DUP	S	Total CN	P	-0.8148	µg/l	5/10/2017 14:17:23	
I3055-01MS	S	Total CN	P	27.9856	µg/l	5/10/2017 14:17:24	
I3055-01MSD	S	Total CN	P	28.1291	µg/l	5/10/2017 14:17:25	
CCV2	S	Total CN	P	253.0142	µg/l	5/10/2017 14:21:06	
CCB2	S	Total CN	P	-1.2309	µg/l	5/10/2017 14:21:07	

LB87368

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

5/10/2017 13:51


Test Total CN

Accepted 5/10/2017 13:51

Factor 947.6
Bias 0.005

Coeff. of det. 0.999773

Errors

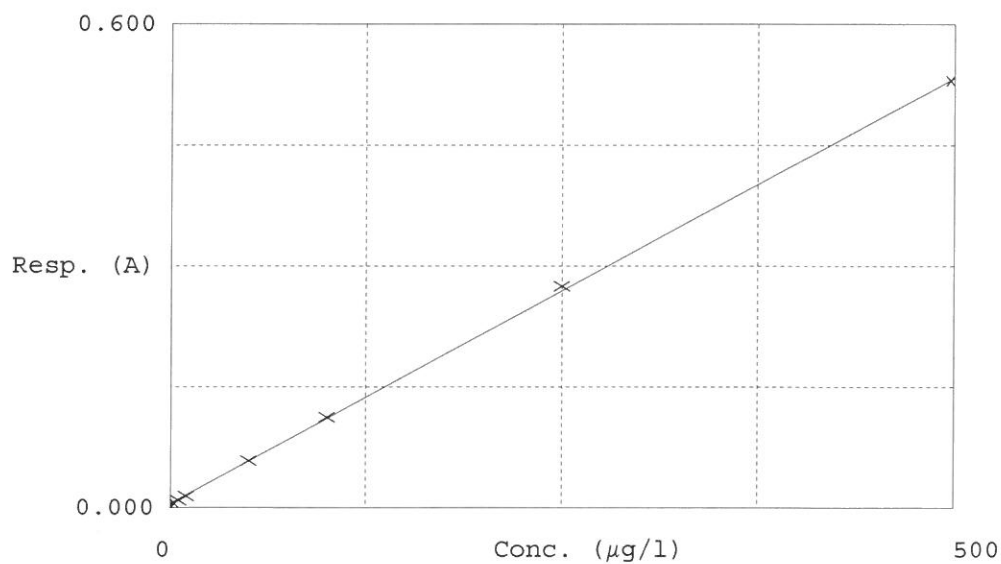

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-1.2671	0.0000	
2	5.0PPBCN	0.009	3.6615	5.0000	
3	10PPBCN	0.014	8.5219	10.0000	
4	50PPBCN	0.058	50.2121	50.0000	
5	100PPBCN	0.112	101.3832	100.0000	
6	250PPBCN	0.275	255.4866	250.0000	
7	500PPBCN	0.530	497.0018	500.0000	