

C88045

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

6/13/2017 10:49

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.194	0.0	0.091	
ICB1	-0.739	0.0	0.004	
CCV1	239.425	0.0	0.227	
CCB1	-0.597	0.0	0.004	
PB99703BL	-0.665	0.0	0.004	
I3624-03	-0.488	0.0	0.004	
I3624-03DUP	-0.543	0.0	0.004	
I3624-06	-0.628	0.0	0.004	
I3628-03	-0.633	0.0	0.004	
I3629-03	-0.423	0.0	0.004	
I3629-07	-0.663	0.0	0.004	
CCV2	251.035	0.0	0.238	
CCB2	-0.440	0.0	0.004	

N	13
Mean	44.449
SD	92.8023
CV%	208.78

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 13 10:45:25 2017

Tue Jun 13 10:48:49 2017

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.8659	µg/l	6/13/2017 9:35:17	
5.0PPBCN	A	Reactive CN	P	4.3973	µg/l	6/13/2017 9:35:18	
10PPBCN	A	Reactive CN	P	9.3327	µg/l	6/13/2017 9:35:19	
50PPBCN	A	Reactive CN	P	49.47	µg/l	6/13/2017 9:35:20	
100PPBCN	A	Reactive CN	P	101.1549	µg/l	6/13/2017 9:35:21	
250PPBCN	A	Reactive CN	P	253.3391	µg/l	6/13/2017 9:35:22	
500PPBCN	A	Reactive CN	P	498.1718	µg/l	6/13/2017 9:35:23	
ICV1	S	Reactive CN	P	93.1939	µg/l	6/13/2017 10:45:25	
ICB1	S	Reactive CN	P	-0.7385	µg/l	6/13/2017 10:45:26	
CCV1	S	Reactive CN	P	239.425	µg/l	6/13/2017 10:45:27	
CCB1	S	Reactive CN	P	-0.5975	µg/l	6/13/2017 10:45:28	
PB99703BL	S	Reactive CN	P	-0.6648	µg/l	6/13/2017 10:45:29	
I3624-03	S	Reactive CN	P	-0.4883	µg/l	6/13/2017 10:45:30	
I3624-03DUP	S	Reactive CN	P	-0.5425	µg/l	6/13/2017 10:45:31	
I3624-06	S	Reactive CN	P	-0.6276	µg/l	6/13/2017 10:45:32	
I3628-03	S	Reactive CN	P	-0.6334	µg/l	6/13/2017 10:45:33	
I3629-03	S	Reactive CN	P	-0.4226	µg/l	6/13/2017 10:45:34	
I3629-07	S	Reactive CN	P	-0.6629	µg/l	6/13/2017 10:45:35	
CCV2	S	Reactive CN	P	251.0349	µg/l	6/13/2017 10:48:48	
CCB2	S	Reactive CN	P	-0.44	µg/l	6/13/2017 10:48:49	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AIC

6/13/2017 9:36


Test Total CN

Accepted 6/13/2017 9:36

Factor 1076
Bias 0.004

Coeff. of det. 0.999914

Errors

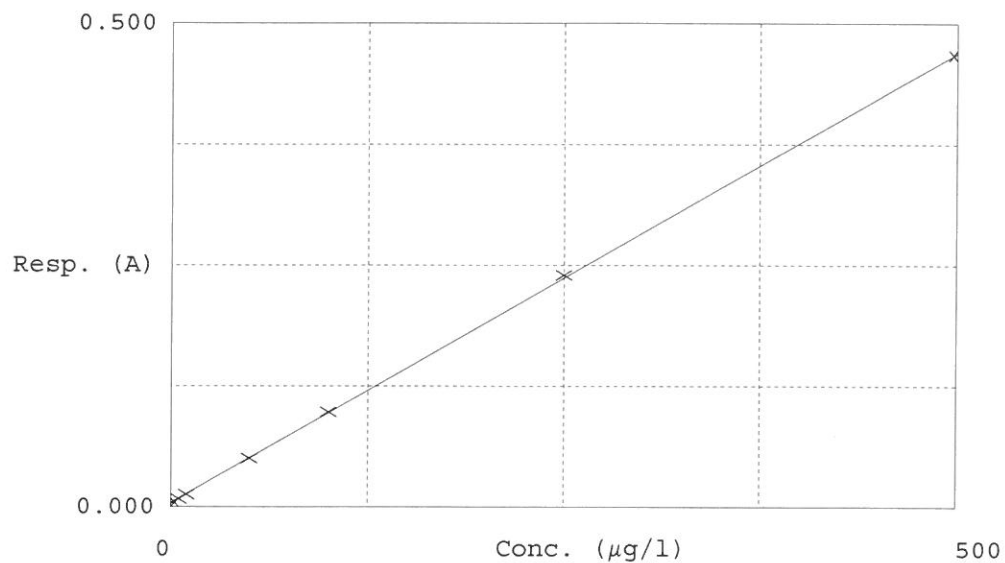

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.8659	0.0000	
2	5.0PPBCN	0.009	4.3973	5.0000	
3	10PPBCN	0.013	9.3327	10.0000	
4	50PPBCN	0.050	49.4700	50.0000	
5	100PPBCN	0.098	101.1549	100.0000	
6	250PPBCN	0.240	253.3391	250.0000	
7	500PPBCN	0.467	498.1718	500.0000	