

6388178

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

6/19/2017 12:19

Test: ^{Reactive} Total CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
ICV1	94.627	0.0	0.092	
ICB1	0.679	0.0	0.004	
CCV1	240.242	0.0	0.227	
CCB1	0.437	0.0	0.004	
PB99883BL	0.211	0.0	0.004	
I3688-19	0.271	0.0	0.004	
I3688-19DUP	0.151	0.0	0.004	
I3688-20	0.391	0.0	0.004	
I3688-21	0.127	0.0	0.004	
I3688-22	-0.070	0.0	0.004	
I3688-23	-0.063	0.0	0.004	
I3688-24	0.410	0.0	0.004	
I3688-25	-0.222	0.0	0.003	
I3688-26	0.283	0.0	0.004	
CCV2	244.553	0.0	0.231	
CCB2	0.799	0.0	0.004	
I3688-27	-0.232	0.0	0.003	
I3688-28	0.137	0.0	0.004	
I3688-29	0.326	0.0	0.004	
I3688-30	-0.215	0.0	0.003	
I3688-31	0.060	0.0	0.004	
I3688-32	0.092	0.0	0.004	
I3688-33	0.202	0.0	0.004	
I3688-34	0.187	0.0	0.004	
I3688-35	-0.152	0.0	0.004	
I3688-36	0.563	0.0	0.004	
CCV3	247.571	0.0	0.233	
CCB3	0.920	0.0	0.005	
I3759-03	0.607	0.0	0.004	
CCV4	250.723	0.0	0.236	
CCB4	0.935	0.0	0.005	

N	31
Mean	34.986
SD	84.2004
CV%	240.67

LB88178

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 19 12:02:42 2017

Mon Jun 19 12:17:01 2017

Alc

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive Cl P		-0.0718	µg/l	6/19/2017 9:00:31	
5.OPPBCN	A	Reactive Cl P		4.5115	µg/l	6/19/2017 9:00:32	
10PPBCN	A	Reactive Cl P		9.627	µg/l	6/19/2017 9:00:33	
50PPBCN	A	Reactive Cl P		48.7962	µg/l	6/19/2017 9:00:34	
100PPBCN	A	Reactive Cl P		100.289	µg/l	6/19/2017 9:00:35	
250PPBCN	A	Reactive Cl P		253.5465	µg/l	6/19/2017 9:00:36	
500PPBCN	A	Reactive Cl P		498.3017	µg/l	6/19/2017 9:00:37	
ICV1	S	Reactive Cl P		94.6272	µg/l	6/19/2017 12:02:42	
ICB1	S	Reactive Cl P		0.679	µg/l	6/19/2017 12:02:43	
CCV1	S	Reactive Cl P		240.2424	µg/l	6/19/2017 12:02:44	
CCB1	S	Reactive Cl P		0.4368	µg/l	6/19/2017 12:02:45	
PB99883BL	S	Reactive Cl P		0.2108	µg/l	6/19/2017 12:02:46	
I3688-19	S	Reactive Cl P		0.2714	µg/l	6/19/2017 12:02:47	
I3688-19DUP	S	Reactive Cl P		0.1512	µg/l	6/19/2017 12:02:48	
I3688-20	S	Reactive Cl P		0.391	µg/l	6/19/2017 12:02:49	
I3688-21	S	Reactive Cl P		0.1275	µg/l	6/19/2017 12:02:50	
I3688-22	S	Reactive Cl P		-0.0705	µg/l	6/19/2017 12:02:51	
I3688-23	S	Reactive Cl P		-0.0629	µg/l	6/19/2017 12:02:52	
I3688-24	S	Reactive Cl P		0.4098	µg/l	6/19/2017 12:10:14	
I3688-25	S	Reactive Cl P		-0.222	µg/l	6/19/2017 12:10:15	
I3688-26	S	Reactive Cl P		0.283	µg/l	6/19/2017 12:10:16	
CCV2	S	Reactive Cl P		244.5535	µg/l	6/19/2017 12:10:17	
CCB2	S	Reactive Cl P		0.7988	µg/l	6/19/2017 12:10:18	
I3688-27	S	Reactive Cl P		-0.2318	µg/l	6/19/2017 12:10:19	
I3688-28	S	Reactive Cl P		0.1372	µg/l	6/19/2017 12:10:20	
I3688-29	S	Reactive Cl P		0.3261	µg/l	6/19/2017 12:10:21	
I3688-30	S	Reactive Cl P		-0.2148	µg/l	6/19/2017 12:10:22	
I3688-31	S	Reactive Cl P		0.0601	µg/l	6/19/2017 12:10:23	
I3688-32	S	Reactive Cl P		0.092	µg/l	6/19/2017 12:10:24	
I3688-33	S	Reactive Cl P		0.2021	µg/l	6/19/2017 12:16:53	
I3688-34	S	Reactive Cl P		0.1874	µg/l	6/19/2017 12:16:54	
I3688-35	S	Reactive Cl P		-0.1523	µg/l	6/19/2017 12:16:55	
I3688-36	S	Reactive Cl P		0.5632	µg/l	6/19/2017 12:16:56	
CCV3	S	Reactive Cl P		247.5711	µg/l	6/19/2017 12:16:57	
CCB3	S	Reactive Cl P		0.92	µg/l	6/19/2017 12:16:58	
I3759-03	S	Reactive Cl P		0.607	µg/l	6/19/2017 12:16:59	
CCV4	S	Reactive Cl P		250.7226	µg/l	6/19/2017 12:17:00	
CCB4	S	Reactive Cl P		0.9349	µg/l	6/19/2017 12:17:01	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

6/19/2017 9:01


Test Total CN

Accepted 6/19/2017 9:01

Factor 1077
Bias 0.004

Coeff. of det. 0.999915

Errors

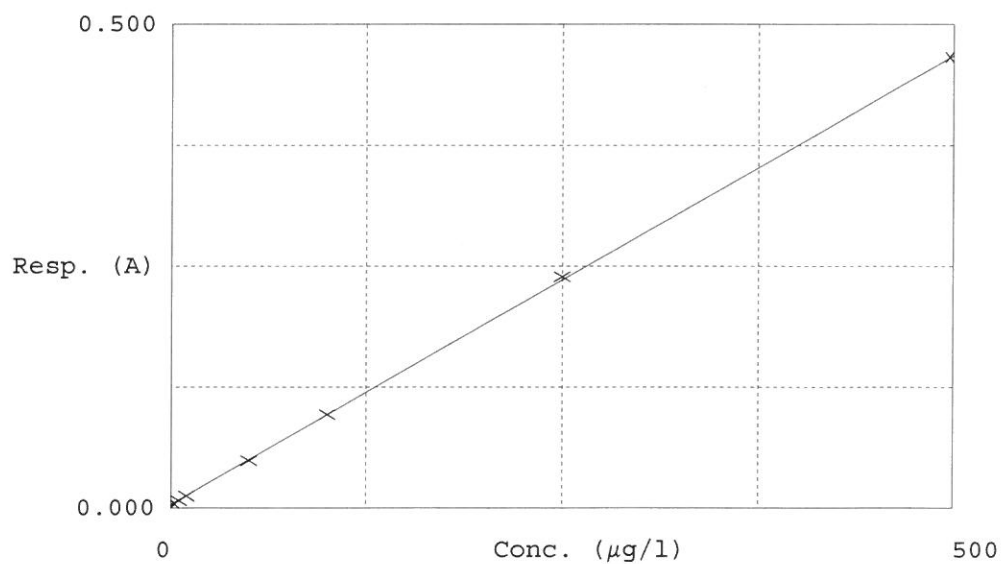

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.0718	0.0000	
2	5.0PPBCN	0.008	4.5115	5.0000	
3	10PPBCN	0.013	9.6270	10.0000	
4	50PPBCN	0.049	48.7962	50.0000	
5	100PPBCN	0.097	100.2890	100.0000	
6	250PPBCN	0.239	253.5465	250.0000	
7	500PPBCN	0.466	498.3017	500.0000	