

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

7/25/2017 13:56

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.912	0.0	0.108	
ICB1	-0.007	0.0	0.003	
CCV1	0.939	0.0	0.111	
CCB1	-0.007	0.0	0.003	
PB100912BL	-0.009	0.0	0.003	
PB100912BS	0.950	0.0	0.113	
I4354-03	0.002	0.0	0.004	
I4354-03DUP	-0.000	0.0	0.004	
I4354-03MS	0.956	0.0	0.113	
I4354-03MSD	0.973	0.0	0.115	
I4402-07	0.016	0.0	0.006	
PB100913BL	0.003	0.0	0.004	
I4407-01	0.008	0.0	0.005	
CCV2	0.968	0.0	0.115	
CCB2	-0.003	0.0	0.004	
I4407-01DUP	0.011	0.0	0.005	
I4407-01MS	0.983	0.0	0.116	
I4407-01MSD	0.970	0.0	0.115	
PB100913BS	1.123	0.0	0.132	
CCV3	0.946	0.0	0.112	
CCB3	-0.013	0.0	0.002	

OK 7/25/17

N	21
Mean	0.463
SD	0.4989
CV%	107.81

Aquakem v. 7.2AQ1

Results from time period:

Tue Jul 25 11:21:08 2017

Tue Jul 25 13:50:52 2017

AK

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0433	mg/l	7/25/2017 11:21:08	
0.1PPM	A	Phenolics-	P	0.131	mg/l	7/25/2017 11:21:09	
0.25PPM	A	Phenolics-	P	0.2329	mg/l	7/25/2017 11:21:10	
0.50PPM	A	Phenolics-	P	0.5154	mg/l	7/25/2017 11:21:11	
1.0PPM	A	Phenolics-	P	0.9611	mg/l	7/25/2017 11:21:12	
2.0PPM	A	Phenolics-	P	2.0164	mg/l	7/25/2017 11:21:13	
ICV1	S	Phenolics-	P	0.9115	mg/l	7/25/2017 13:24:48	
ICB1	S	Phenolics-	P	-0.0074	mg/l	7/25/2017 13:24:49	
CCV1	S	Phenolics-	P	0.9392	mg/l	7/25/2017 13:24:50	
CCB1	S	Phenolics-	P	-0.007	mg/l	7/25/2017 13:24:51	
PB100912BL	S	Phenolics-	P	-0.0094	mg/l	7/25/2017 13:24:52	
PB100912BS	S	Phenolics-	P	0.9497	mg/l	7/25/2017 13:24:53	
I4354-03	S	Phenolics-	P	0.0021	mg/l	7/25/2017 13:24:54	
I4354-03DUP	S	Phenolics-	P	0	mg/l	7/25/2017 13:24:55	
I4354-03MS	S	Phenolics-	P	0.9556	mg/l	7/25/2017 13:24:56	
I4354-03MSD	S	Phenolics-	P	0.9732	mg/l	7/25/2017 13:24:57	
I4402-07	S	Phenolics-	P	0.0161	mg/l	7/25/2017 13:24:58	
CCV2	S	Phenolics-	P	0.9676	mg/l	7/25/2017 13:32:25	
CCB2	S	Phenolics-	P	-0.0028	mg/l	7/25/2017 13:32:26	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : PIC

7/25/2017 11:37


Test Phenolics-

Accepted 7/25/2017 11:37

Factor 8.733
Bias 0.004

Coeff. of det. 0.998813

Errors

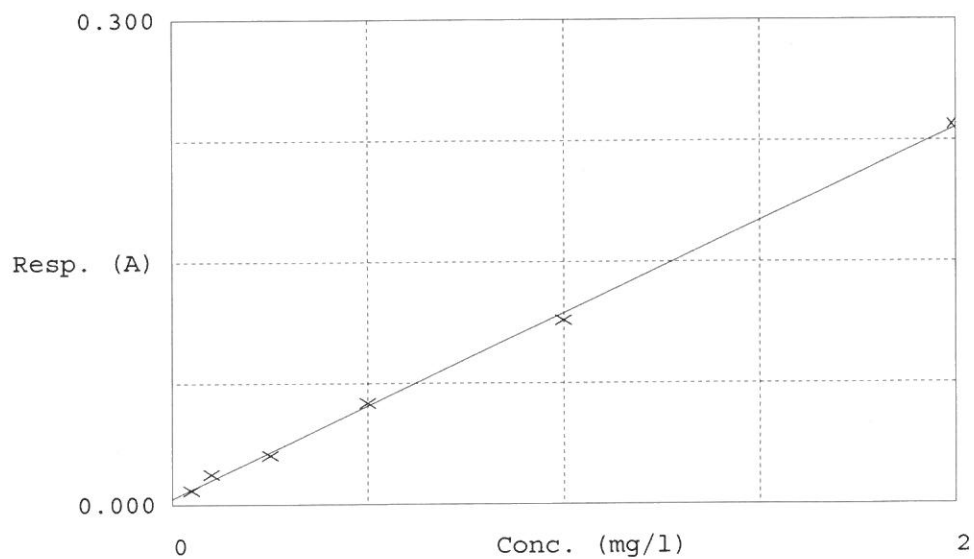

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.009	0.0433	0.0500	
2	Phenol-2	0.019	0.1310	0.1000	
3	Phenol-2	0.031	0.2329	0.2500	
4	Phenol-2	0.063	0.5154	0.5000	
5	Phenol-2	0.114	0.9611	1.0000	
6	Phenol-2	0.235	2.0164	2.0000	