

CB 89055

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

7/27/2017 9:56

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.136	0.0	0.106	
ICB1	0.039	0.0	0.004	
CCV1	242.958	0.0	0.261	
CCB1	-0.003	0.0	0.004	
PB100811BL	0.045	0.0	0.004	
PB100811BS	96.901	0.0	0.107	
I4252-01	0.393	0.0	0.005	
I4252-01DUP	-0.240	0.0	0.004	
I4346-30	677.277	0.0	0.721	Test limit high
CCV2	248.990	0.0	0.268	
CCB2	0.571	0.0	0.005	
MIDPB100811	249.557	0.0	0.268	
I4252-01MS	42.703	0.0	0.049	
I4252-01MSD	42.508	0.0	0.049	
I4346-30DLX2	362.782	0.0	0.388	
CCV3	250.911	0.0	0.270	
CCB3	-0.281	0.0	0.004	

N	17
Mean	135.956
SD	184.4943
CV%	135.70

CB 89055

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 27 08:41:24 2017

Thu Jul 27 09:46:09 2017

AL

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.5413	µg/l	7/27/2017 8:41:24	
5.OPPBCN	A	Total CN	P	4.3857	µg/l	7/27/2017 8:41:25	
10PPBCN	A	Total CN	P	9.8557	µg/l	7/27/2017 8:41:26	
50PPBCN	A	Total CN	P	50.0023	µg/l	7/27/2017 8:41:27	
100PPBCN	A	Total CN	P	101.6029	µg/l	7/27/2017 8:41:28	
250PPBCN	A	Total CN	P	250.0129	µg/l	7/27/2017 8:41:29	
500PPBCN	A	Total CN	P	499.6818	µg/l	7/27/2017 8:41:30	
ICV1	S	Total CN	P	96.1357	µg/l	7/27/2017 9:14:26	
ICB1	S	Total CN	P	0.0387	µg/l	7/27/2017 9:14:27	
CCV1	S	Total CN	P	242.9577	µg/l	7/27/2017 9:14:28	
CCB1	S	Total CN	P	-0.0031	µg/l	7/27/2017 9:14:29	
PB100811BL	S	Total CN	P	0.0451	µg/l	7/27/2017 9:14:30	
PB100811BS	S	Total CN	P	96.9007	µg/l	7/27/2017 9:14:31	
I4252-01	S	Total CN	P	0.3933	µg/l	7/27/2017 9:14:33	
I4252-01DUP	S	Total CN	P	-0.2399	µg/l	7/27/2017 9:14:34	
I4346-30	S	Total CN	P	677.277	µg/l	7/27/2017 9:21:06	
CCV2	S	Total CN	P	248.9898	µg/l	7/27/2017 9:21:08	
CCB2	S	Total CN	P	0.571	µg/l	7/27/2017 9:21:09	
MIDPB100811	S	Total CN	P	249.5566	µg/l	7/27/2017 9:46:03	
I4252-01MS	S	Total CN	P	42.7034	µg/l	7/27/2017 9:46:04	
I4252-01MSD	S	Total CN	P	42.5076	µg/l	7/27/2017 9:46:05	
I4346-30DLX2	S	Total CN	P	362.7822	µg/l	7/27/2017 9:46:07	
CCV3	S	Total CN	P	250.9106	µg/l	7/27/2017 9:46:08	
CCB3	S	Total CN	P	-0.2807	µg/l	7/27/2017 9:46:09	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : A2K

7/27/2017 8:42


Test Total CN

Accepted 7/27/2017 8:42

Factor 945.3
Bias 0.004

Coeff. of det. 0.999984

Errors

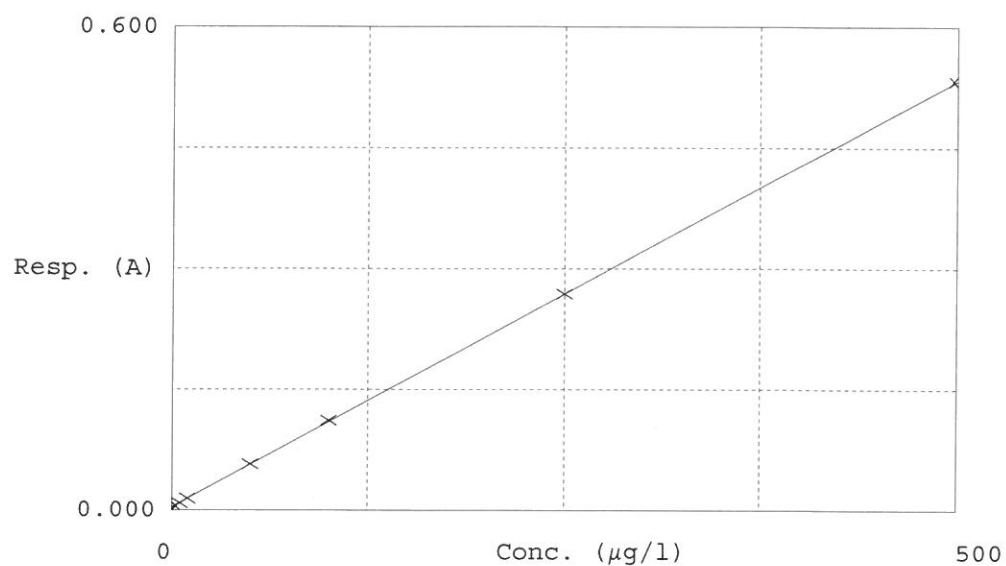

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.5413	0.0000	
2	5.0PPBCN	0.009	4.3857	5.0000	
3	10PPBCN	0.015	9.8557	10.0000	
4	50PPBCN	0.057	50.0023	50.0000	
5	100PPBCN	0.112	101.6029	100.0000	
6	250PPBCN	0.269	250.0129	250.0000	
7	500PPBCN	0.533	499.6818	500.0000	