

=====

Calibration results

Aquakem 7.2AQ1

2
2B89489
Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DP

8/15/2017 12:15


Test Phenolics-

Accepted 8/15/2017 12:15

Factor 8.947
Bias 0.003

Coeff. of det. 0.999726

Errors

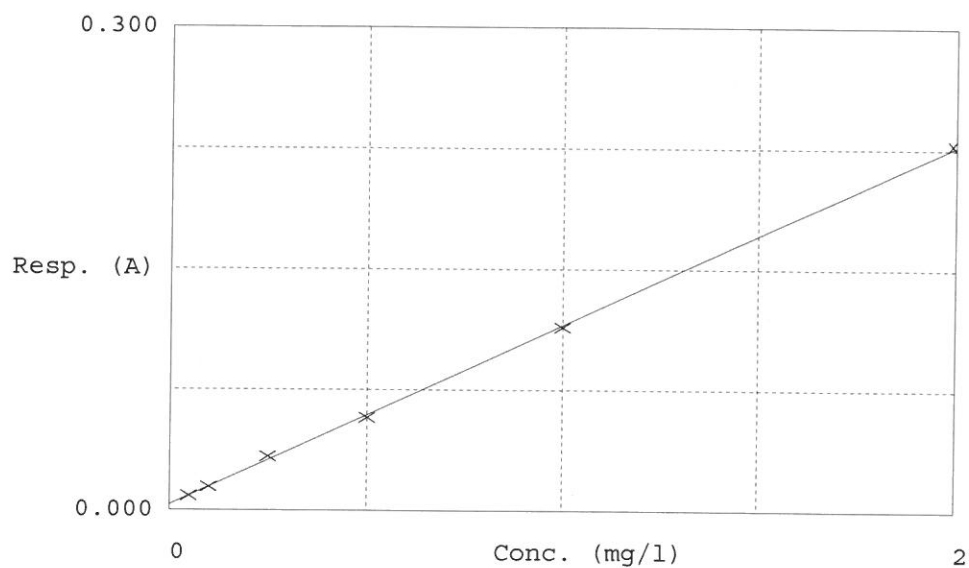

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.009	0.0494	0.0500	
2	Phenol-2	0.015	0.0999	0.1000	
3	Phenol-2	0.034	0.2696	0.2500	
4	Phenol-2	0.058	0.4858	0.5000	
5	Phenol-2	0.114	0.9885	1.0000	
6	Phenol-2	0.228	2.0069	2.0000	

LB89489

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 15 12:10:51 2017

Tue Aug 15 13:27:32 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0494	mg/l	8/15/2017 12:10:51	
0.1PPM	A	Phenolics-	P	0.0999	mg/l	8/15/2017 12:10:52	
0.25PPM	A	Phenolics-	P	0.2696	mg/l	8/15/2017 12:10:53	
0.50PPM	A	Phenolics-	P	0.4858	mg/l	8/15/2017 12:10:54	
1.0PPM	A	Phenolics-	P	0.9885	mg/l	8/15/2017 12:10:55	
2.0PPM	A	Phenolics-	P	2.0069	mg/l	8/15/2017 12:10:56	
ICV1	S	Phenolics-	P	1.0209	mg/l	8/15/2017 12:43:05	
ICB1	S	Phenolics-	P	0.0017	mg/l	8/15/2017 12:43:06	
CCV1	S	Phenolics-	P	1.0173	mg/l	8/15/2017 13:23:36	
CCB1	S	Phenolics-	P	0.0035	mg/l	8/15/2017 13:23:37	
PB101538BL	S	Phenolics-	P	0.0005	mg/l	8/15/2017 13:23:38	
PB101538BS	S	Phenolics-	P	1.0257	mg/l	8/15/2017 13:23:39	
I4736-13	S	Phenolics-	P	-0.0004	mg/l	8/15/2017 13:23:40	
I4736-13DUP	S	Phenolics-	P	-0.0028	mg/l	8/15/2017 13:23:41	
I4736-13MS	S	Phenolics-	P	1.0142	mg/l	8/15/2017 13:23:42	
I4736-13MSD	S	Phenolics-	P	1.0085	mg/l	8/15/2017 13:23:43	
I4736-14	S	Phenolics-	P	-0.0026	mg/l	8/15/2017 13:23:44	
CCV2	S	Phenolics-	P	1.0045	mg/l	8/15/2017 13:27:31	
CCB2	S	Phenolics-	P	0.0061	mg/l	8/15/2017 13:27:32	

=====

Test results

Aquakem 7.2AQ1

2B89489
Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DP

8/15/2017 13:30

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.021	0.0	0.118	
ICB1	0.002	0.0	0.004	
CCV1	1.017	0.0	0.117	
CCB1	0.004	0.0	0.004	
PB101538BL	0.001	0.0	0.003	
PB101538BS	1.026	0.0	0.118	
I4736-13	-0.000	0.0	0.003	
I4736-13DUP	-0.003	0.0	0.003	
I4736-13MS	1.014	0.0	0.117	
I4736-13MSD	1.008	0.0	0.116	
I4736-14	-0.003	0.0	0.003	
CCV2	1.004	0.0	0.116	
CCB2	0.006	0.0	0.004	

N	13
Mean	0.469
SD	0.5263
CV%	112.22