

UB96697

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DP

10/10/2017 13:49

Test: ~~Total~~ CN

Reactive
ug/l

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.987	0.0	0.101	
ICB1	0.657	0.0	0.004	
CCV1	247.770	0.0	0.250	
CCB1	0.958	0.0	0.004	
PB103134BL	0.872	0.0	0.004	
I5766-02	0.670	0.0	0.004	
I5766-02DUP	1.403	0.0	0.005	
PB103133BL	0.619	0.0	0.004	
I5763-04	-0.134	0.0	0.003	
I5763-04DUP	0.845	0.0	0.004	
I5765-03	0.475	0.0	0.004	
I5766-07	1.236	0.0	0.004	
CCV2	254.017	0.0	0.256	
CCB2	1.601	0.0	0.005	

N	14
Mean	43.498
SD	91.5829
CV%	210.54

LB90697

Aquakem v. 7.2AQ1

Results from time period:

Tue Oct 10 13:40:51 2017

Tue Oct 10 13:47:09 2017

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	REACTIVE CN	P	0.9482	µg/l	10/10/2017 9:25:42	
5.0PPBCN	A	REACTIVE CN	P	4.8693	µg/l	10/10/2017 9:25:43	
10PPBCN	A	REACTIVE CN	P	9.3978	µg/l	10/10/2017 9:25:44	
50PPBCN	A	REACTIVE CN	P	47.6698	µg/l	10/10/2017 9:25:45	
100PPBCN	A	REACTIVE CN	P	100.0878	µg/l	10/10/2017 9:25:46	
250PPBCN	A	REACTIVE CN	P	253.5966	µg/l	10/10/2017 9:25:47	
500PPBCN	A	REACTIVE CN	P	498.4305	µg/l	10/10/2017 9:25:48	
ICV1	S	REACTIVE CN	P	97.9873	µg/l	10/10/2017 13:40:52	
ICB1	S	REACTIVE CN	P	0.6573	µg/l	10/10/2017 13:40:54	
CCV1	S	REACTIVE CN	P	247.7699	µg/l	10/10/2017 13:40:56	
CCB1	S	REACTIVE CN	P	0.9577	µg/l	10/10/2017 13:40:57	
PB103134BL	S	REACTIVE CN	P	0.8721	µg/l	10/10/2017 13:41:00	
I5766-02	S	REACTIVE CN	P	0.6703	µg/l	10/10/2017 13:41:01	
I5766-02DUP	S	REACTIVE CN	P	1.4028	µg/l	10/10/2017 13:47:02	
PB103133BL	S	REACTIVE CN	P	0.6186	µg/l	10/10/2017 13:47:03	
I5763-04	S	REACTIVE CN	P	-0.1337	µg/l	10/10/2017 13:47:04	
I5763-04DUP	S	REACTIVE CN	P	0.8449	µg/l	10/10/2017 13:47:05	
I5765-03	S	REACTIVE CN	P	0.4754	µg/l	10/10/2017 13:47:06	
I5766-07	S	REACTIVE CN	P	1.2361	µg/l	10/10/2017 13:47:07	
CCV2	S	REACTIVE CN	P	254.0171	µg/l	10/10/2017 13:47:08	
CCB2	S	REACTIVE CN	P	1.601	µg/l	10/10/2017 13:47:09	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : DP

10/10/2017 9:27


Test Reactive
~~Total CN~~

Accepted 10/10/2017 9:27

Factor 1005
 Bias 0.003

Coeff. of det. 0.999892

Errors

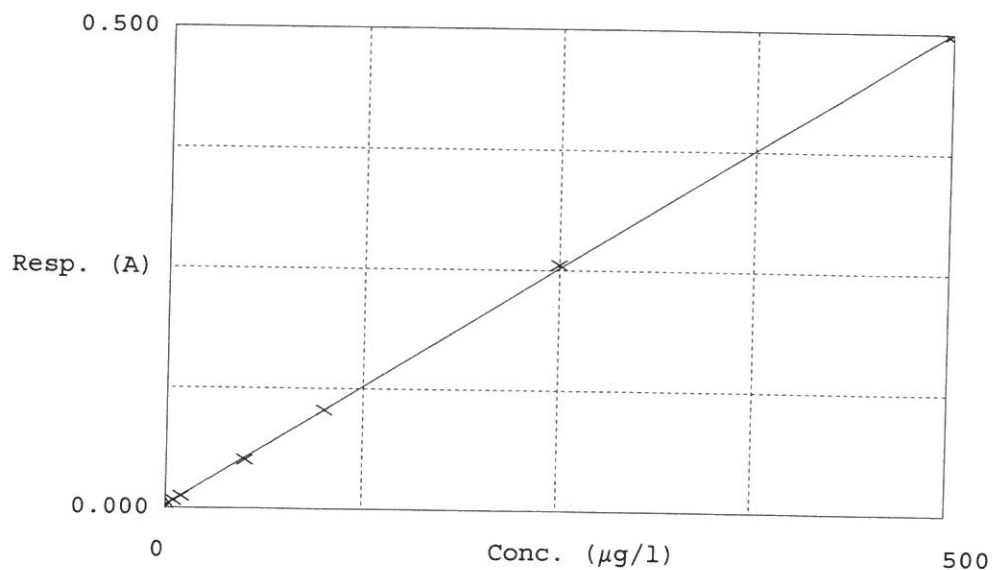

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.9482	0.0000	
2	5.0PPBCN	0.008	4.8693	5.0000	
3	10PPBCN	0.012	9.3978	10.0000	
4	50PPBCN	0.051	47.6698	50.0000	
5	100PPBCN	0.103	100.0878	100.0000	
6	250PPBCN	0.255	253.5966	250.0000	
7	500PPBCN	0.499	498.4305	500.0000	