

LB90908

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DP

10/18/2017 11:38


Test Phenolics-

Accepted 10/18/2017 11:38

Factor 8.74
Bias 0.004

Coeff. of det. 0.999805

Errors

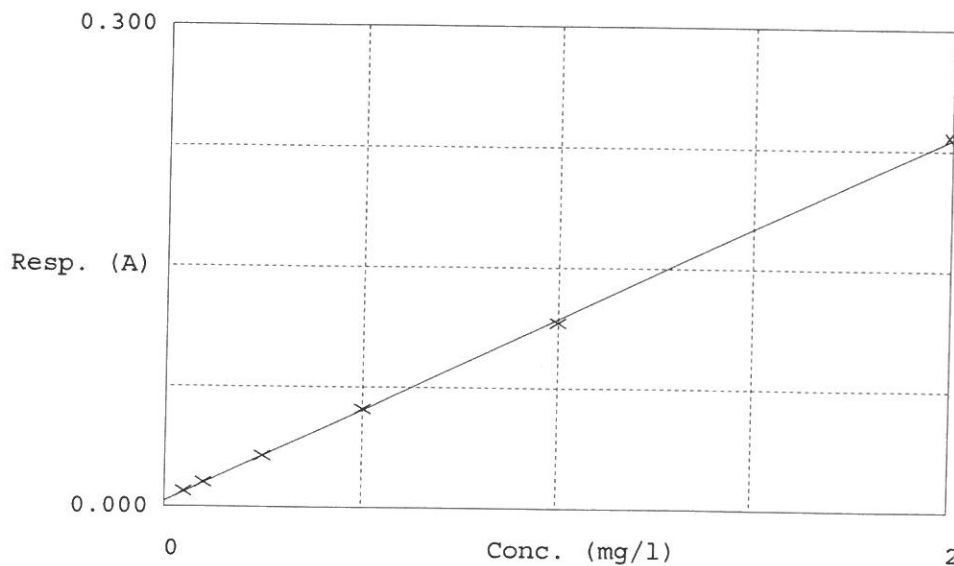

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.010	0.0539	0.0500	
2	Phenol-2	0.015	0.1032	0.1000	
3	Phenol-2	0.032	0.2492	0.2500	
4	Phenol-2	0.061	0.5054	0.5000	
5	Phenol-2	0.116	0.9797	1.0000	
6	Phenol-2	0.233	2.0086	2.0000	

LB90908

Aquakem v. 7.2AQ1

Results from time period:

Wed Oct 18 11:34:58 2017

Wed Oct 18 12:21:57 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0539	mg/l	10/18/2017 11:34:58	
0.1PPM	A	Phenolics-	P	0.1032	mg/l	10/18/2017 11:34:59	
0.25PPM	A	Phenolics-	P	0.2492	mg/l	10/18/2017 11:35:00	
0.50PPM	A	Phenolics-	P	0.5054	mg/l	10/18/2017 11:35:01	
1.0PPM	A	Phenolics-	P	0.9797	mg/l	10/18/2017 11:35:02	
2.0PPM	A	Phenolics-	P	2.0086	mg/l	10/18/2017 11:35:03	
ICV1	S	Phenolics-	P	1.0008	mg/l	10/18/2017 12:06:30	
ICB1	S	Phenolics-	P	0.0005	mg/l	10/18/2017 12:06:32	
CCV1	S	Phenolics-	P	1.0333	mg/l	10/18/2017 12:06:33	
CCB1	S	Phenolics-	P	-0.0013	mg/l	10/18/2017 12:06:36	
PB103387BL	S	Phenolics-	P	-0.0004	mg/l	10/18/2017 12:16:37	
PB103387BS	S	Phenolics-	P	0.9994	mg/l	10/18/2017 12:16:38	
I5901-01	S	Phenolics-	P	0.002	mg/l	10/18/2017 12:16:39	
I5901-01DUP	S	Phenolics-	P	0.0026	mg/l	10/18/2017 12:16:40	
I5901-01MS	S	Phenolics-	P	0.9257	mg/l	10/18/2017 12:16:41	
I5901-01MSD	S	Phenolics-	P	0.9116	mg/l	10/18/2017 12:16:42	
I5901-03	S	Phenolics-	P	0.001	mg/l	10/18/2017 12:21:53	
I5901-05	S	Phenolics-	P	0.0038	mg/l	10/18/2017 12:21:54	
I5901-06	S	Phenolics-	P	0.0061	mg/l	10/18/2017 12:21:55	
CCV2	S	Phenolics-	P	1.0224	mg/l	10/18/2017 12:21:56	
CCB2	S	Phenolics-	P	0.0008	mg/l	10/18/2017 12:21:57	

LB90908

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : DP

10/18/2017 12:23

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.001	0.0	0.118	
ICB1	0.001	0.0	0.004	
CCV1	1.033	0.0	0.122	
CCB1	-0.001	0.0	0.003	
PB103216BL	0.001	0.0	0.004	
PB103216BS	1.017	0.0	0.120	
I5822-02	0.009	0.0	0.005	
I5822-02DUP	0.007	0.0	0.004	
I5822-01MS	0.880	0.0	0.104	
I5822-02MSD	0.883	0.0	0.105	
PB103387BL	-0.000	0.0	0.003	
PB103387BS	0.999	0.0	0.118	
I5901-01	0.002	0.0	0.004	
I5901-01DUP	0.003	0.0	0.004	
I5901-01MS	0.926	0.0	0.109	
I5901-01MSD	0.912	0.0	0.108	
I5901-03	0.001	0.0	0.004	
I5901-05	0.004	0.0	0.004	
I5901-06	0.006	0.0	0.004	
CCV2	1.022	0.0	0.121	
CCB2	0.001	0.0	0.004	

10/18/17

N 21
 Mean 0.415
 SD 0.4889
 CV% 117.93