

CB9BTH

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/3/2017 16:08

Test: Total CN Mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.524	0.0	0.094	
ICB1	0.078	0.0	0.004	
CCV1	245.937	0.0	0.233	
CCB1	0.123	0.0	0.004	
PB103950BL	-0.295	0.0	0.003	
I6289-02	-0.411	0.0	0.003	
I6289-02DUP	-0.178	0.0	0.003	
I6299-02	-0.194	0.0	0.003	
PB103956BL	-0.152	0.0	0.003	
I6294-02	-0.236	0.0	0.003	
I6294-02DUP	-0.061	0.0	0.003	
I6296-02	-0.256	0.0	0.003	
CCV2	253.553	0.0	0.240	
CCB2	-0.168	0.0	0.003	

N	14
Mean	42.519
SD	91.5572
CV%	215.33

Aquakem v. 7.2AQ1

Results from time period:

AS

Fri Nov 03 15:56:45 2017

Fri Nov 03 16:02:34 2017

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.433	µg/l	11/3/2017 10:28:34	
5.OPPBCN	A	Reactive CN	P	4.7648	µg/l	11/3/2017 10:28:35	
10PPBCN	A	Reactive CN	P	9.6572	µg/l	11/3/2017 10:28:36	
50PPBCN	A	Reactive CN	P	50.0702	µg/l	11/3/2017 10:28:37	
100PPBCN	A	Reactive CN	P	101.0255	µg/l	11/3/2017 10:28:38	
250PPBCN	A	Reactive CN	P	250.2367	µg/l	11/3/2017 10:28:39	
500PPBCN	A	Reactive CN	P	499.6787	µg/l	11/3/2017 10:28:40	
ICV1	S	Reactive CN	P	97.5238	µg/l	11/3/2017 15:56:46	
ICB1	S	Reactive CN	P	0.0776	µg/l	11/3/2017 15:56:48	
CCV1	S	Reactive CN	P	245.9366	µg/l	11/3/2017 15:56:50	
CCB1	S	Reactive CN	P	0.1229	µg/l	11/3/2017 15:56:51	
PB103950BL	S	Reactive CN	P	-0.2948	µg/l	11/3/2017 15:56:53	
I6289-02	S	Reactive CN	P	-0.4107	µg/l	11/3/2017 15:56:54	
I6289-02DUP	S	Reactive CN	P	-0.1782	µg/l	11/3/2017 15:56:55	
I6299-02	S	Reactive CN	P	-0.1943	µg/l	11/3/2017 16:02:28	
PB103956BL	S	Reactive CN	P	-0.1523	µg/l	11/3/2017 16:02:29	
I6294-02	S	Reactive CN	P	-0.236	µg/l	11/3/2017 16:02:30	
I6294-02DUP	S	Reactive CN	P	-0.0613	µg/l	11/3/2017 16:02:31	
I6296-02	S	Reactive CN	P	-0.2563	µg/l	11/3/2017 16:02:32	
CCV2	S	Reactive CN	P	253.5527	µg/l	11/3/2017 16:02:33	
CCB2	S	Reactive CN	P	-0.1679	µg/l	11/3/2017 16:02:34	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/3/2017 10:33


Test Total CN

Accepted 11/3/2017 10:33

Factor 1074
Bias 0.003

Coeff. of det. 0.999992

Errors

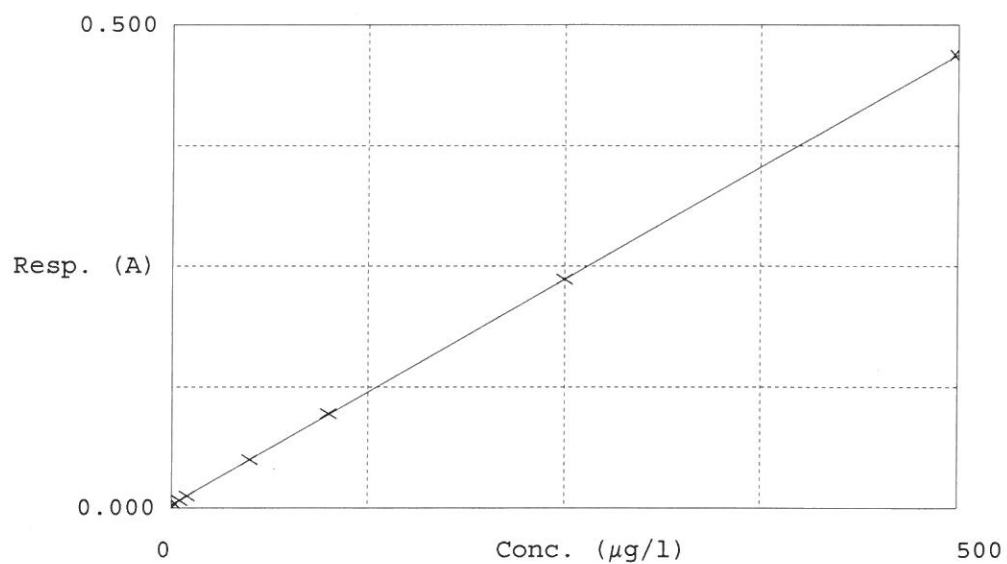

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.4330	0.0000	
2	5.0PPBCN	0.008	4.7648	5.0000	
3	10PPBCN	0.012	9.6572	10.0000	
4	50PPBCN	0.050	50.0702	50.0000	
5	100PPBCN	0.098	101.0255	100.0000	
6	250PPBCN	0.237	250.2367	250.0000	
7	500PPBCN	0.469	499.6787	500.0000	