

LB91439

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/8/2017 10:42

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.384	0.0	0.102	
ICB1	-1.690	0.0	0.003	
CCV1	252.162	0.0	0.256	
CCB1	-1.492	0.0	0.003	
PB104046BL	-1.773	0.0	0.003	
I6300-02	-2.101	0.0	0.003	
I6300-02DUP	-2.046	0.0	0.003	
I6311-02	-1.772	0.0	0.003	
I6359-04	-1.787	0.0	0.003	
PB104048BL	-1.704	0.0	0.003	
I6351-02	-1.828	0.0	0.003	
I6351-02DUP	-1.620	0.0	0.003	
I6358-02	-1.817	0.0	0.003	
CCV2	252.693	0.0	0.257	
CCB2	-1.646	0.0	0.003	

N	15
Mean	38.731
SD	90.4197
CV%	233.46

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 08 09:09:47 2017

Wed Nov 08 10:39:37 2017

AK

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-1.6855	µg/l	11/8/2017 9:55:03	
5.OPPBCN	A	Reactive CN	P	3.2684	µg/l	11/8/2017 9:55:04	
10PPBCN	A	Reactive CN	P	8.1604	µg/l	11/8/2017 9:55:05	
50PPBCN	A	Reactive CN	P	49.8605	µg/l	11/8/2017 9:55:06	
100PPBCN	A	Reactive CN	P	100.8546	µg/l	11/8/2017 9:55:07	
250PPBCN	A	Reactive CN	P	259.2891	µg/l	11/8/2017 9:55:08	
500PPBCN	A	Reactive CN	P	495.2526	µg/l	11/8/2017 9:55:09	
ICV1	S	Reactive CN	P	97.3836	µg/l	11/8/2017 10:33:20	
ICB1	S	Reactive CN	P	-1.6899	µg/l	11/8/2017 10:33:21	
CCV1	S	Reactive CN	P	252.1622	µg/l	11/8/2017 10:33:24	
CCB1	S	Reactive CN	P	-1.4918	µg/l	11/8/2017 10:33:25	
PB104046BL	S	Reactive CN	P	-1.7732	µg/l	11/8/2017 10:33:27	
I6300-02	S	Reactive CN	P	-2.1012	µg/l	11/8/2017 10:33:28	
I6300-02DUP	S	Reactive CN	P	-2.0457	µg/l	11/8/2017 10:33:29	
I6311-02	S	Reactive CN	P	-1.7724	µg/l	11/8/2017 10:39:30	
I6359-04	S	Reactive CN	P	-1.7873	µg/l	11/8/2017 10:39:31	
PB104048BL	S	Reactive CN	P	-1.7036	µg/l	11/8/2017 10:39:32	
I6351-02	S	Reactive CN	P	-1.8278	µg/l	11/8/2017 10:39:33	
I6351-02DUP	S	Reactive CN	P	-1.6201	µg/l	11/8/2017 10:39:34	
I6358-02	S	Reactive CN	P	-1.8173	µg/l	11/8/2017 10:39:35	
CCV2	S	Reactive CN	P	252.6932	µg/l	11/8/2017 10:39:36	
CCB2	S	Reactive CN	P	-1.646	µg/l	11/8/2017 10:39:37	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/8/2017 9:55


Test Total CN

Accepted 11/8/2017 9:55

Factor 1004
Bias 0.005

Coeff. of det. 0.999422

Errors

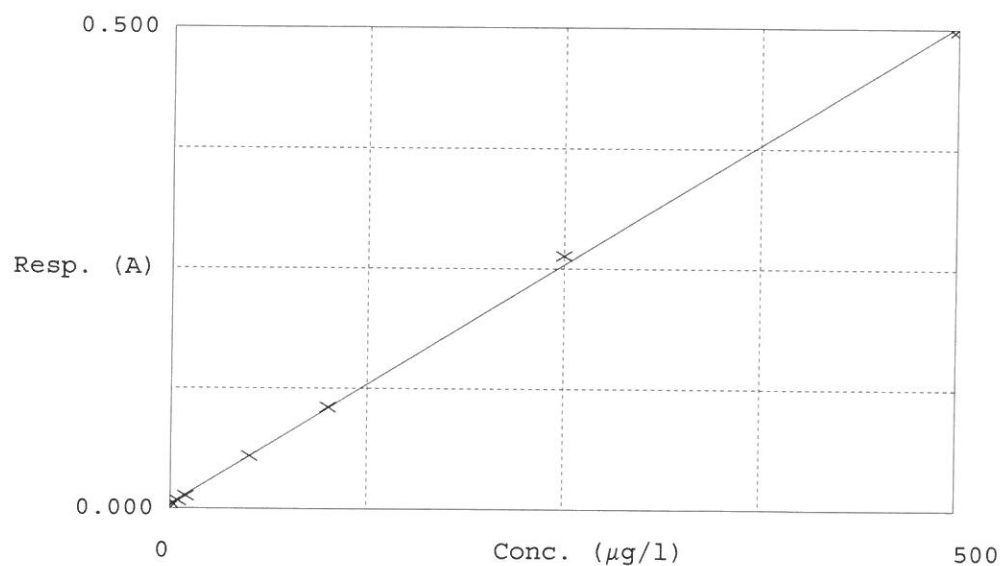

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.6855	0.0000	
2	5.0PPBCN	0.008	3.2684	5.0000	
3	10PPBCN	0.013	8.1604	10.0000	
4	50PPBCN	0.055	49.8605	50.0000	
5	100PPBCN	0.105	100.8546	100.0000	
6	250PPBCN	0.263	259.2891	250.0000	
7	500PPBCN	0.498	495.2526	500.0000	