

=====

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/8/2017 12:13

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.034	0.0	0.116	
ICB1	0.005	0.0	0.010	
CCV1	1.049	0.0	0.117	
CCB1	0.001	0.0	0.009	
PB104695BL	0.000	0.0	0.009	
PB104695BS	1.021	0.0	0.114	
I6693-01	0.004	0.0	0.009	
I6693-01DUP	0.002	0.0	0.009	
I6693-01MS	0.924	0.0	0.105	
I6693-01MSD	0.916	0.0	0.104	
I6693-02	0.001	0.0	0.009	
I6693-03	0.003	0.0	0.009	
I6693-04	0.001	0.0	0.009	
I6720-01	0.003	0.0	0.009	
CCV2	1.062	0.0	0.119	
CCB2	-0.004	0.0	0.009	
I6720-02	0.006	0.0	0.010	
I6720-03	0.004	0.0	0.009	
CCV3	1.061	0.0	0.119	
CCB3	-0.009	0.0	0.008	

N 20
Mean 0.354
SD 0.4946
CV% 139.64

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Dec 08 09:57:39 2017

Fri Dec 08 12:10:26 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0509	mg/l	12/8/2017 9:57:39	
0.1PPM	A	Phenolics-	P	0.1001	mg/l	12/8/2017 9:57:40	
0.25PPM	A	Phenolics-	P	0.2463	mg/l	12/8/2017 9:57:41	
0.50PPM	A	Phenolics-	P	0.5027	mg/l	12/8/2017 9:57:42	
1.0PPM	A	Phenolics-	P	1.0005	mg/l	12/8/2017 9:57:43	
2.0PPM	A	Phenolics-	P	1.9995	mg/l	12/8/2017 9:57:44	
ICV1	S	Phenolics-	P	1.0335	mg/l	12/8/2017 12:03:33	
ICB1	S	Phenolics-	P	0.0049	mg/l	12/8/2017 12:03:34	
CCV1	S	Phenolics-	P	1.0489	mg/l	12/8/2017 12:03:35	
CCB1	S	Phenolics-	P	0.001	mg/l	12/8/2017 12:03:36	
PB104695BL	S	Phenolics-	P	0.0004	mg/l	12/8/2017 12:03:37	
PB104695BS	S	Phenolics-	P	1.0205	mg/l	12/8/2017 12:03:38	
I6693-01	S	Phenolics-	P	0.0036	mg/l	12/8/2017 12:03:39	
I6693-01DUP	S	Phenolics-	P	0.0023	mg/l	12/8/2017 12:03:40	
I6693-01MS	S	Phenolics-	P	0.924	mg/l	12/8/2017 12:03:41	
I6693-01MSD	S	Phenolics-	P	0.9162	mg/l	12/8/2017 12:03:42	
I6693-02	S	Phenolics-	P	0.0015	mg/l	12/8/2017 12:03:43	
I6693-03	S	Phenolics-	P	0.0032	mg/l	12/8/2017 12:03:44	
I6693-04	S	Phenolics-	P	0.0012	mg/l	12/8/2017 12:10:19	
I6720-01	S	Phenolics-	P	0.0032	mg/l	12/8/2017 12:10:20	
CCV2	S	Phenolics-	P	1.0617	mg/l	12/8/2017 12:10:21	
CCB2	S	Phenolics-	P	-0.0042	mg/l	12/8/2017 12:10:22	
I6720-02	S	Phenolics-	P	0.0056	mg/l	12/8/2017 12:10:23	
I6720-03	S	Phenolics-	P	0.0039	mg/l	12/8/2017 12:10:24	
CCV3	S	Phenolics-	P	1.0608	mg/l	12/8/2017 12:10:25	
CCB3	S	Phenolics-	P	-0.0087	mg/l	12/8/2017 12:10:26	

LB 92033

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

12/8/2017 10:09

Test Phenolics-


Accepted 12/8/2017 10:09

Factor 9.684

Bias 0.009

Coeff. of det. 0.999992

Errors

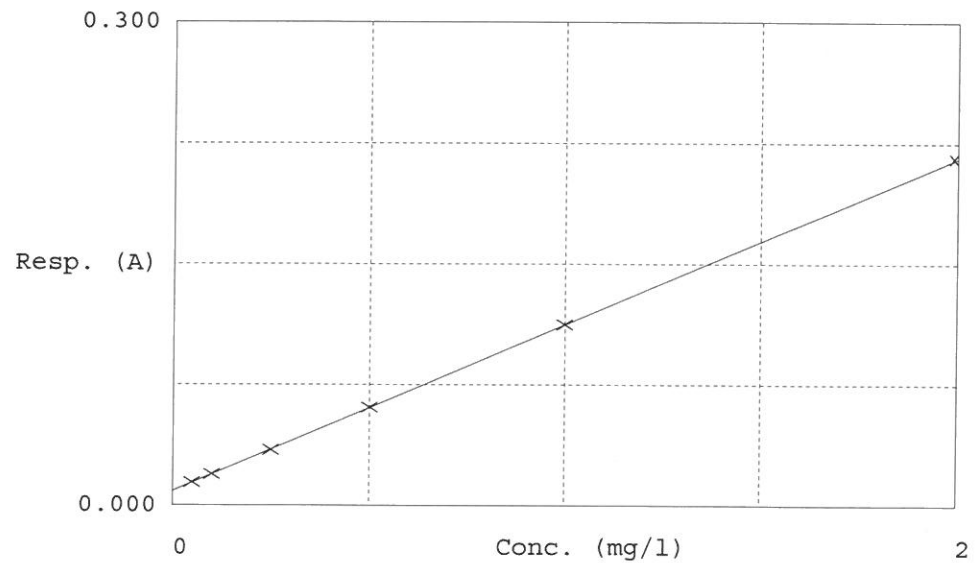

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.014	0.0509	0.0500	
2	Phenol-2	0.019	0.1001	0.1000	
3	Phenol-2	0.035	0.2463	0.2500	
4	Phenol-2	0.061	0.5027	0.5000	
5	Phenol-2	0.112	1.0005	1.0000	
6	Phenol-2	0.216	1.9995	2.0000	