

LB92163

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/14/2017 13:17

Test: *Reactive*
Total CN *ug/d*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.894	0.0	0.092	
ICB1	0.437	0.0	0.004	
CCV1	240.685	0.0	0.229	
CCB1	0.766	0.0	0.004	
PB105036BL	0.391	0.0	0.004	
I6678-02	0.023	0.0	0.003	
I6678-02DUP	-0.140	0.0	0.003	
I6679-04	0.061	0.0	0.003	
I6679-06	0.067	0.0	0.003	
I6679-08	0.053	0.0	0.003	
I6889-03	-0.206	0.0	0.003	
I6889-05	0.228	0.0	0.004	
CCV2	245.390	0.0	0.234	
CCB2	0.456	0.0	0.004	

N	14
Mean	41.650
SD	88.9533
CV%	213.57

AS

Aquakem v. 7.2AQ1

Results from time period:

Thu Dec 14 12:29:19 2017

Thu Dec 14 13:01:17 2017

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.2219	µg/l	12/14/2017 12:29:19	
5.0PPBCN	A	Reactive CN	P	5.1169	µg/l	12/14/2017 12:29:20	
10PPBCN	A	Reactive CN	P	9.8192	µg/l	12/14/2017 12:29:21	
50PPBCN	A	Reactive CN	P	51.0747	µg/l	12/14/2017 12:29:22	
100PPBCN	A	Reactive CN	P	99.2192	µg/l	12/14/2017 12:29:23	
250PPBCN	A	Reactive CN	P	248.9939	µg/l	12/14/2017 12:29:24	
500PPBCN	A	Reactive CN	P	500.5542	µg/l	12/14/2017 12:29:25	
ICV1	S	Reactive CN	P	94.8944	µg/l	12/14/2017 12:55:28	
ICB1	S	Reactive CN	P	0.4374	µg/l	12/14/2017 12:55:30	
CCV1	S	Reactive CN	P	240.6846	µg/l	12/14/2017 12:55:33	
CCB1	S	Reactive CN	P	0.7661	µg/l	12/14/2017 12:55:35	
PB105036BL	S	Reactive CN	P	0.3907	µg/l	12/14/2017 12:55:36	
I6678-02	S	Reactive CN	P	0.0228	µg/l	12/14/2017 12:55:37	
I6678-02DUP	S	Reactive CN	P	-0.1397	µg/l	12/14/2017 12:55:38	
I6679-04	S	Reactive CN	P	0.0607	µg/l	12/14/2017 13:01:11	
I6679-06	S	Reactive CN	P	0.067	µg/l	12/14/2017 13:01:12	
I6679-08	S	Reactive CN	P	0.0529	µg/l	12/14/2017 13:01:13	
I6889-03	S	Reactive CN	P	-0.2058	µg/l	12/14/2017 13:01:14	
I6889-05	S	Reactive CN	P	0.2282	µg/l	12/14/2017 13:01:15	
CCV2	S	Reactive CN	P	245.3898	µg/l	12/14/2017 13:01:16	
CCB2	S	Reactive CN	P	0.4564	µg/l	12/14/2017 13:01:17	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/14/2017 12:30


Test Total CN

Accepted 12/14/2017 12:30

Factor 1066
Bias 0.003

Coeff. of det. 0.999985

Errors

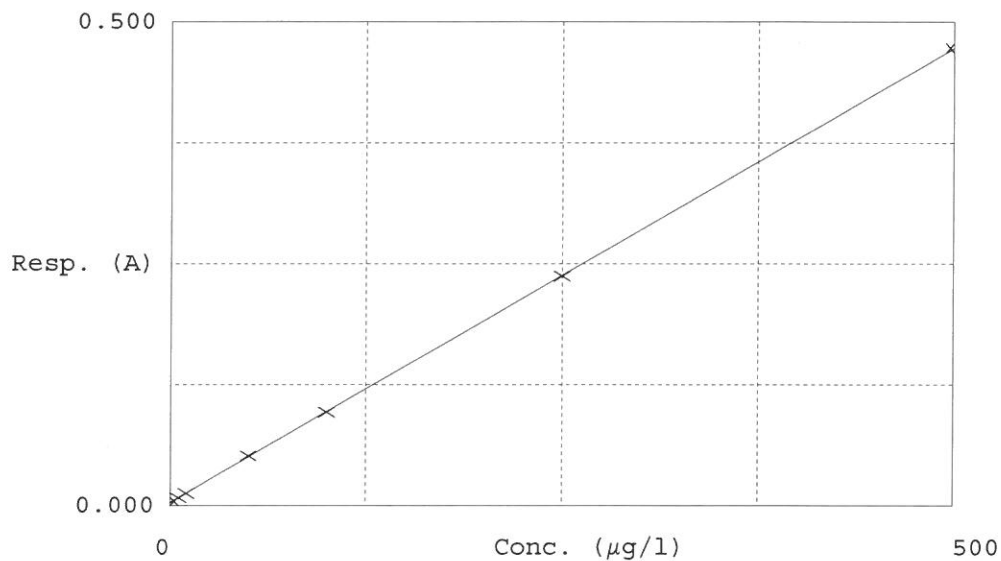

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.2219	0.0000	
2	5.0PPBCN	0.008	5.1169	5.0000	
3	10PPBCN	0.013	9.8192	10.0000	
4	50PPBCN	0.051	51.0747	50.0000	
5	100PPBCN	0.096	99.2192	100.0000	
6	250PPBCN	0.237	248.9939	250.0000	
7	500PPBCN	0.473	500.5542	500.0000	