

1892185

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/15/2017 12:07

Test: Total CN *My Id*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.019	0.0	0.094	
ICB1	0.462	0.0	0.004	
CCV1	242.869	0.0	0.231	
CCB1	0.449	0.0	0.004	
PB105062BL	1.162	0.0	0.005	
PB105062BS	95.921	0.0	0.093	
LOWPB105062	9.758	0.0	0.013	
HIGHPB105062	483.300	0.0	0.456	
I6680-11	0.587	0.0	0.004	
I6680-11DUP	0.333	0.0	0.004	
I6680-11MS	34.263	0.0	0.036	
I6680-11MSD	33.911	0.0	0.035	
I6680-13	0.489	0.0	0.004	
I6680-15	1.128	0.0	0.005	
CCV2	244.873	0.0	0.233	
CCB2	0.575	0.0	0.004	
I6680-17	0.670	0.0	0.004	
I6744-05	1.689	0.0	0.005	
I6911-01	0.726	0.0	0.004	
I6919-01	1.082	0.0	0.005	
CCV3	249.232	0.0	0.237	
CCB3	0.242	0.0	0.004	

N	22
Mean	68.170
SD	125.9734
CV%	184.79

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Dec 15 11:19:40 2017

Fri Dec 15 12:06:40 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.0912	µg/l	12/15/2017 11:19:40	
5.OPPBCN	A	Total CN	P	4.8553	µg/l	12/15/2017 11:19:41	
10PPBCN	A	Total CN	P	9.6182	µg/l	12/15/2017 11:19:42	
50PPBCN	A	Total CN	P	50.6021	µg/l	12/15/2017 11:19:43	
100PPBCN	A	Total CN	P	99.3818	µg/l	12/15/2017 11:19:44	
250PPBCN	A	Total CN	P	251.1224	µg/l	12/15/2017 11:19:45	
500PPBCN	A	Total CN	P	499.5113	µg/l	12/15/2017 11:19:46	
ICV1	S	Total CN	P	96.0185	µg/l	12/15/2017 11:53:48	
ICB1	S	Total CN	P	0.4615	µg/l	12/15/2017 11:53:49	
CCV1	S	Total CN	P	242.8691	µg/l	12/15/2017 11:53:52	
CCB1	S	Total CN	P	0.4493	µg/l	12/15/2017 11:53:53	
PB105062BL	S	Total CN	P	1.162	µg/l	12/15/2017 11:53:55	
PB105062BS	S	Total CN	P	95.9205	µg/l	12/15/2017 11:53:56	
LOWPB105062	S	Total CN	P	9.7578	µg/l	12/15/2017 11:53:57	
HIGHPB105062	S	Total CN	P	483.2998	µg/l	12/15/2017 12:01:20	
I6680-11	S	Total CN	P	0.5867	µg/l	12/15/2017 12:01:21	
I6680-11DUP	S	Total CN	P	0.3333	µg/l	12/15/2017 12:01:22	
I6680-11MS	S	Total CN	P	34.2629	µg/l	12/15/2017 12:01:23	
I6680-11MSD	S	Total CN	P	33.9108	µg/l	12/15/2017 12:01:24	
I6680-13	S	Total CN	P	0.4887	µg/l	12/15/2017 12:01:25	
I6680-15	S	Total CN	P	1.1275	µg/l	12/15/2017 12:01:26	
CCV2	S	Total CN	P	244.8726	µg/l	12/15/2017 12:01:27	
CCB2	S	Total CN	P	0.5753	µg/l	12/15/2017 12:01:28	
I6680-17	S	Total CN	P	0.6696	µg/l	12/15/2017 12:01:29	
I6744-05	S	Total CN	P	1.6889	µg/l	12/15/2017 12:01:30	
I6911-01	S	Total CN	P	0.7259	µg/l	12/15/2017 12:06:35	
I6919-01	S	Total CN	P	1.082	µg/l	12/15/2017 12:06:36	
CCV3	S	Total CN	P	249.2321	µg/l	12/15/2017 12:06:37	
CCB3	S	Total CN	P	0.2421	µg/l	12/15/2017 12:06:38	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/15/2017 11:22


Test Total CN

Accepted 12/15/2017 11:22

Factor 1068
Bias 0.004

Coeff. of det. 0.999988

Errors

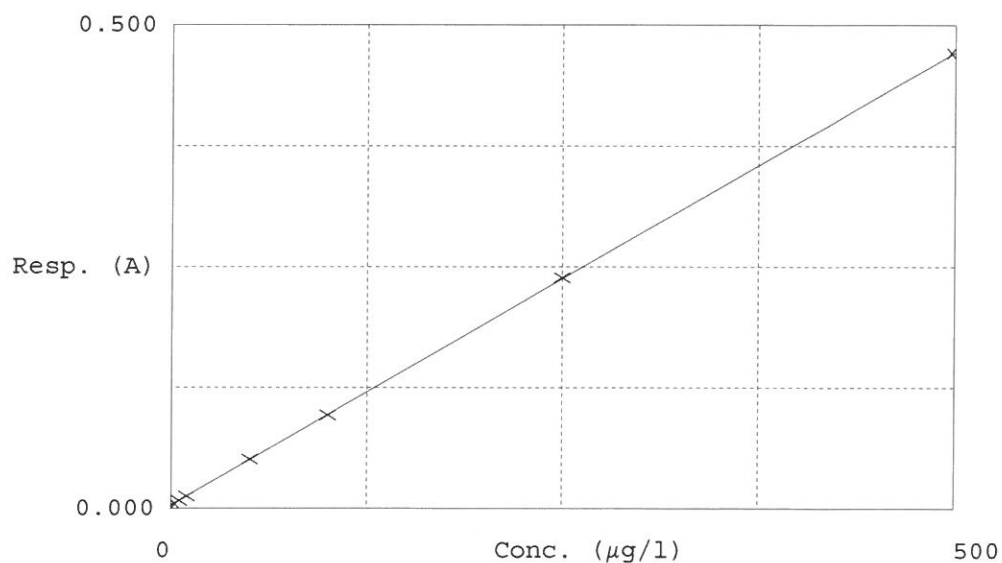

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.0912	0.0000	
2	5.0PPBCN	0.008	4.8553	5.0000	
3	10PPBCN	0.013	9.6182	10.0000	
4	50PPBCN	0.051	50.6021	50.0000	
5	100PPBCN	0.097	99.3818	100.0000	
6	250PPBCN	0.239	251.1224	250.0000	
7	500PPBCN	0.471	499.5113	500.0000	